

Aug 17, 2020

Agarose Gel Electrophoresis-Chem 584



Forked from [Agarose Gel Electrophoresis](#)

DOI

dx.doi.org/10.17504/protocols.io.bjvnkn5e


Ken Christensen¹, Addgene The Nonprofit Plasmid Repository²

¹Brigham Young University; ²Addgene



Ken Christensen

Brigham Young University



OPEN  ACCESS



DOI: dx.doi.org/10.17504/protocols.io.bjvnkn5e

External link: <https://www.addgene.org/protocols/gel-electrophoresis/>

Protocol Citation: Ken Christensen, Addgene The Nonprofit Plasmid Repository 2020. Agarose Gel Electrophoresis-Chem 584 . protocols.io <https://dx.doi.org/10.17504/protocols.io.bjvnkn5e>

License: This is an open access protocol distributed under the terms of the [Creative Commons Attribution License](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited

Protocol status: Working

We use this protocol and it's working

Created: August 17, 2020

Last Modified: August 17, 2020

Protocol Integer ID: 40590

Abstract

This protocol is for agarose gel electrophoresis. To see the full abstract and additional resources, visit the [Addgene protocol page](#).



Guidelines

Analyzing your gel

Using the DNA ladder in the first lane as a guide (the manufacturer's instruction will tell you the size of each band), you can infer the size of the DNA in your sample lanes. For more details on doing diagnostic digests and how to interpret them please see the [Diagnostic Digest](#) page.

Purifying DNA from your gel

If you are conducting certain procedures, such as molecular cloning, you will need to purify the DNA away from the agarose gel. For instructions on how to do this, visit the [Gel Purification](#) page.

Tips and FAQ

■ How do you get better resolution of bands?

A few simple ways to increase the resolution (crispness) of your DNA bands include: a) running the gel at a lower voltage for a longer period of time; b) using a wider/thinner gel comb; or c) loading less DNA into the well. Another method for visualizing very short DNA fragments is polyacrylamide gel electrophoresis (PAGE), which is typically used to separate 5 - 500 bp fragments.

■ How do you get better separation of bands?

If you have similarly sized bands that are running too close together, you can adjust the agarose percentage of the gel to get better separation. A higher percentage agarose gel will help resolve smaller bands from each other, and a lower percentage gel will help separate larger bands.

■ 10% Rule:

For each sample you want to load on a gel, make 10% more volume than needed because several microliters can be lost in pipetting. For example, if you want to load 1.0 µg in 10 µL, make 1.1 µg in 11 µL.



Materials

Equipment

- Casting tray
- Well combs
- Voltage source
- Gel box
- UV light source
- Microwave

Reagents



- TAE ([recipe here](#))
- Agarose
- Ethidium bromide (stock concentration of 10 mg/mL)

Pouring a Standard 1% Agarose Gel


- 1 Measure  .6 g of agarose.

Note

Pro-Tip

Agarose gels are commonly used in concentrations of 0.7%-2% depending on the size of bands needed to be separated -see FAQ section of this protocol. Simply adjust the mass of agarose in a given volume to make gels of other agarose concentrations (e.g.,  2 g of agarose in  100 mL of TAE will make a 2% gel).

- 2 Mix agarose powder with  60 mL 1xTAE in a microwavable flask. **See TAE Recipe.**

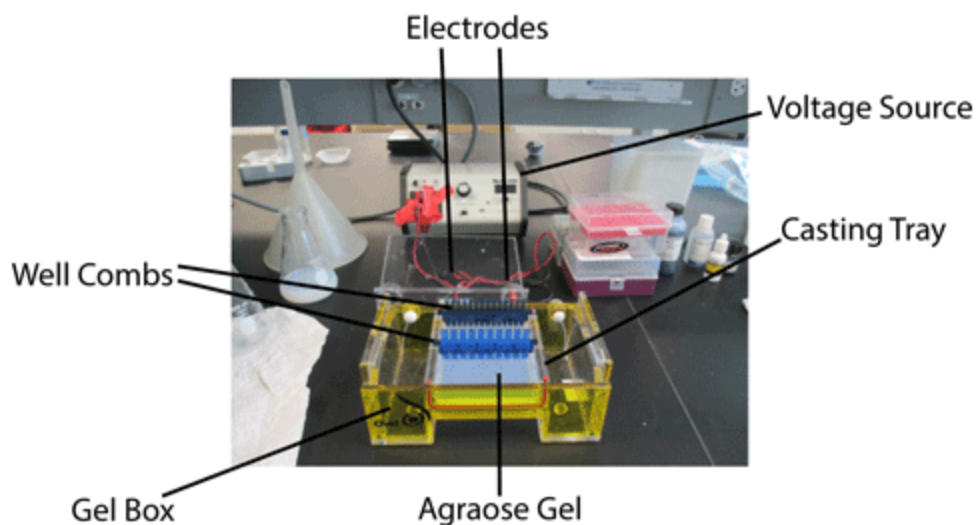



Note

Pro-Tip

TBE can be used instead of TAE, labs usually use one or the other, but there is very little difference between the two.

**Note**



Note, make sure to use the same buffer as the one in the gel box (do not mix different buffers and do not use water).






- 3 Microwave for  00:01:00 to  00:03:00 until the agarose is completely dissolved (but do not overboil the solution, as some of the buffer will evaporate and thus alter the final percentage of agarose in the gel. Many people prefer to microwave in pulses, swirling the flask occasionally as the solution heats up.)

Safety information

CAUTION: HOT! Be careful stirring, eruptive boiling can occur.

Note***Pro-Tip***






It is a good idea to microwave for  00:00:30 -  00:00:45 , stop and swirl, and then continue towards a boil. Keep an eye on it the solution has a tendency to boil over. Placing saran wrap over the top of the flask can help with this, but is not necessary if you pay close attention.

- 4 Let agarose solution cool down to about  50 °C (about when you can comfortably keep your hand on the flask), about  00:05:00 .
- 5 Add Midori Green (25,000x) to a final concentration of 1x (about  2 µL -  3 µL of lab stock solution per  60 mL gel). EtBr binds to the DNA and allows you to visualize the DNA under ultraviolet (UV) light.
- 6 Pour the agarose into a gel tray with the well comb in place.

Note


Pro-Tip

Pour slowly to avoid bubbles which will disrupt the gel. Any bubbles can be pushed away from the well comb or towards the sides/edges of the gel with a pipette tip.

- 7 Place newly poured gel at  4 °C for  00:10:00 -  00:15:00 OR let sit at room temperature for  00:20:00 -  00:30:00 , until it has completely solidified.


Note

Pro-Tip

If you are in a hurry, the gel will set more quickly if you place the gel tray at  4 °C earlier so that it is already cold when the gel is poured into it.

Loading Samples and Running an Agarose Gel

- 8 Add loading buffer (6x Purple Loading Dye from NEB) to each of your DNA samples.

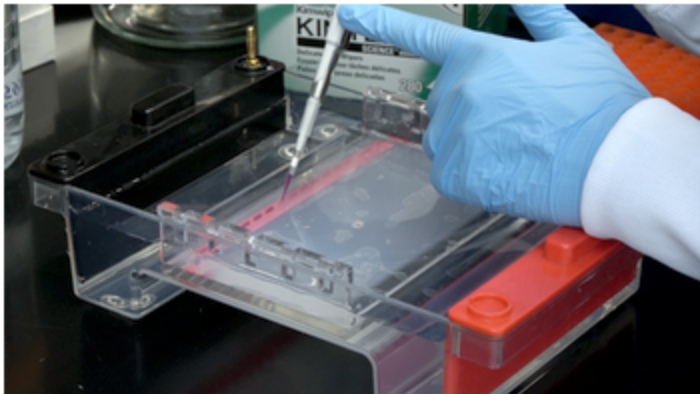

loading a gel

Note


Note: Loading buffer serves two purposes: 1) it provides a visible dye that helps with gel loading and allows you to gauge how far the DNA has migrated; 2) it contains a high percentage of glycerol that increases the density of your DNA sample causing it settle to the bottom of the gel well, instead of diffusing in the buffer.

- 9 Once solidified, place the agarose gel into the gel box (electrophoresis unit).
- 10 Fill gel box with 1xTAE (or TBE) until the gel is covered.
- 11 Carefully load a molecular weight ladder into the first lane of the gel.

Note

Note, when loading the sample in the well, maintain positive pressure on the sample to prevent bubbles or buffer from entering the tip. Place the very top of the tip of the pipette into the buffer just above the well. Very slowly and steadily, push the sample out and watch as the sample fills the well. After all of the sample is unloaded, push the pipettor to the second stop and carefully raise the pipette straight out of the buffer.

- 12 Carefully load your samples into the additional wells of the gel.

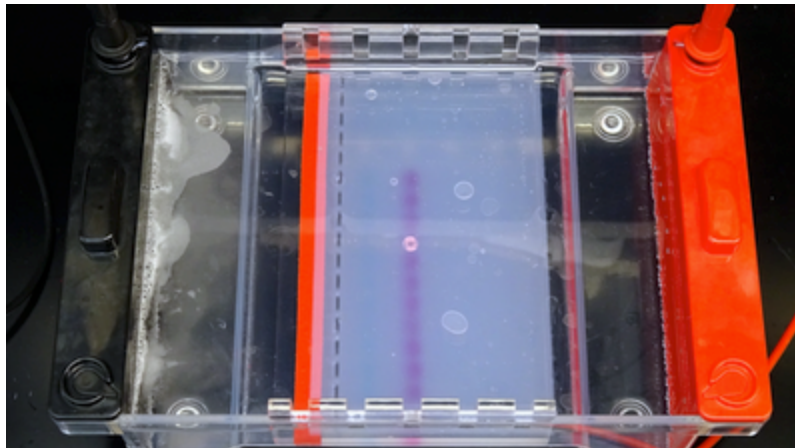

gel loaded with samples

- 13 Run the gel at 80-150 V until the dye line is approximately 75-80% of the way down the gel. A typical run time is about 🕒 01:00:00 - 🕒 01:30:00 , depending on the gel concentration and voltage.

**Note**

Note: Black is negative, red is positive. The DNA is negatively charged and will run towards the positive electrode. Always Run to Red.

- 14 Turn OFF power, disconnect the electrodes from the power source, and then carefully remove the gel from the gel box.
- 15 Using any device that has UV light, visualize your DNA fragments. The fragments of DNA are usually referred to as 'bands' due to their appearance on the gel.

Safety information

CAUTION: When using UV light, protect your skin by wearing safety goggles or a face shield, gloves and a lab coat.

Note***Pro-Tip***

If you will be purifying the DNA for later use, use long-wavelength UV and expose for as little time as possible to minimize damage to the DNA.