



Nov 11, 2017 Version 3

🌐 Human Parechovirus A real-time RT-PCR ["Nix assay"; 2008-2015] V.3

DOI

dx.doi.org/10.17504/protocols.io.krpcv5n


Ian M Mackay¹

¹The University of Queensland



Ian M Mackay

The University of Queensland



OPEN ACCESS



DOI: dx.doi.org/10.17504/protocols.io.krpcv5n

Protocol Citation: Ian M Mackay 2017. Human Parechovirus A real-time RT-PCR ["Nix assay"; 2008-2015]. **protocols.io** <https://dx.doi.org/10.17504/protocols.io.krpcv5n>

Manuscript citation:

The oligonucleotides used in this assay have been previously published.

Nix WA, Maher K, Johansson ES, Niklasson B, Lindberg AM, Pallansch MA, Oberste MS. Detection of all known parechoviruses by real-time PCR. J Clin Microbiol.46(8):2519-2524.

License: This is an open access protocol distributed under the terms of the **Creative Commons Attribution License**, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited

Protocol status: Working

We used this protocol in our group and it worked.

Created: November 11, 2017

Last Modified: March 27, 2018

Protocol Integer ID: 8719

Keywords: parechovirus, respiratory virus, RT-PCR, real-time PCR, rtPCR



Abstract

I and my team used this assay between 2008-2015; we dubbed it the "Nix assay". It targets the 5'UTR and employs quite degenerate oligos.

In silico sequence alignments indicated the oligonucleotides could theoretically detect at least HPeV 1-7, 17 and 18. However during a period of assay comparison, another assay (see link below), the "Benschop assay" ([J.Clin.Virol. 2008. 41\(2\):69-74](#)), was found to produce more sigmoidal and higher curves and 1-5 cycle improvements to C_T values when compared among the sample sample extract set.

Guidelines

- This protocol assumes the user is familiar with working in a laboratory, with PCR, the thermocycler and software used to run it
- This protocol should be re-evaluated if being used with different reagents, if the oligonucleotide sequences are changed or if the cycling conditions are altered

Materials

STEP MATERIALS

 SuperScript™ III Platinum™ One-Step qRT-PCR Kit [Life Technologies Catalog #11732088](#)

 SuperScript™ III Platinum™ One-Step qRT-PCR Kit [Life Technologies Catalog #11732088](#)

Protocol materials

 SuperScript™ III Platinum™ One-Step qRT-PCR Kit [Life Technologies Catalog #11732088](#)


 SuperScript™ III Platinum™ One-Step qRT-PCR Kit [Life Technologies Catalog #11732088](#)

 SuperScript™ III Platinum™ One-Step qRT-PCR Kit [Life Technologies Catalog #11732088](#)

Oligonucleotides...

1	Name	5'-3' oligonucleotide sequence
	AN345_panHPeV/LV (sense primer)	GTAACASWWGCCTCTGGGSCCAAAAG
	AN344_panHPeV/LV (antisense probe)	GGCCCCWGRTCAGATCCAYAGT
	AN257_HPeV/LV (probe)	FAM-CCTRYGGGTACCTYCWGGGCATCCTTC-BHQ1

Reagents

- 2  SuperScript™ III Platinum™ One-Step qRT-PCR Kit Life Technologies Catalog #11732088

Reaction setup...

- 3 Below is the reaction setup for a single RT-PCR reaction.

Ideally, this work is conduct in a laboratory separate to any space used to perform PCR, molecular cloning or the analysis or high concentration DNA.

This volume has been used in 0.1-0.2ml tubes or various other connected tube configurations such as 100-place rings.

Multiply this according to the number of reactions you will need, remembering to include a positive control and at least two non-template controls (NTCs)

You may also need to allow some extra volume, depending on the method used to pipette mix into tubes for the run. For example, some robot-loaded tubes can require two reaction 'dead volumes'.

Reagent (stock concentration)	Vol (μL) / reaction	Final concentration
Nuclease free water	4.47	N/A
AN345_panHPeV/LV (200pmol/ul)	0.03	300nM
AN344_panHPeV/LV (200pmol/ul)	0.03	300nM
AN257_HPeV/LV FAM-BHQ1 (100pmol/ul)	0.03	150nM
2X Reaction Mix ¹	10	1X
Rox Reference Dye 25mM ¹	0.04	50nM
SuperScript® III/Platinum® Taq Mix ¹	0.4	1X



Template extract RNA	5	N/A
Final volume	20µl	

1

SuperScript® III Platinum® One-Step qRT-PCR Kit, Cat No. 11732088

Amplification...

- 4 This assay has been optimized and validated for use with a Rotor-Gene 6000 or Rotor-Gene Q thermal cycler.

The cycling conditions are as follows:

RT-PCR		
50°C	5min	
95°C	2min	
95°C	3s	40X
60°C	30s*	

*Florescence acquisition step

Result calling...

- 5 The definition used for a satisfactory positive result from a real-time fluorogenic PCR should include each of the following:
1. A **sigmoidal curve** – the trace travels horizontally, curves upward, continues in an exponential rise, curves and reaches a horizontal plateau phase
 2. A **suitable level of fluorescence** intensity as measured in comparison to a positive control (y-axis)
 3. A defined threshold (C_T) value which the fluorescent curve has clearly exceeded (Fig.1 arrow) and which sits early in the log-linear phase
 4. A flat or non-sigmoidal curve or a curve that crosses the threshold with a C_T value >40 cycles is considered a negative result
 5. No template controls (NTCs; water instead of specimen extract) should not produce a curve

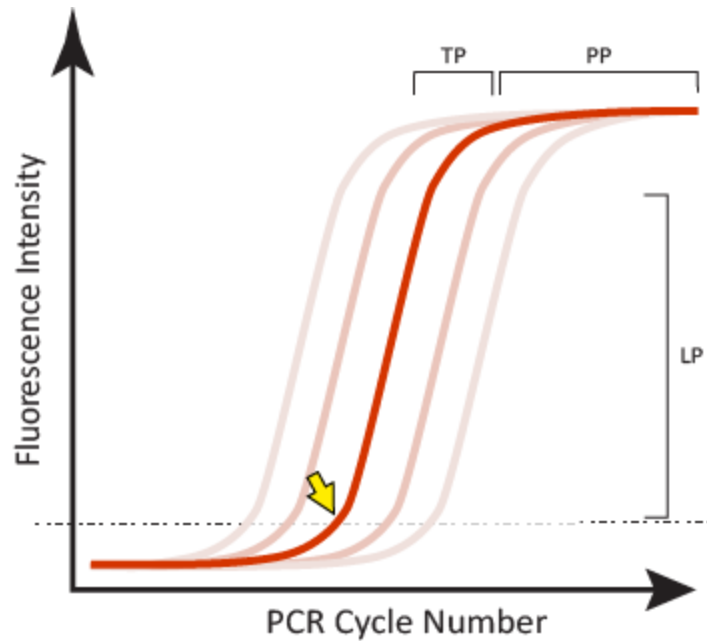


Figure 1. Examples of satisfactory sigmoidal amplification curve shape when considering an assay's fluorescent signal output. The crossing point or threshold cycle (C_T) is indicated (yellow arrow); it is the value at which fluorescence levels surpass a predefined (usually set during validation, or arbitrary) threshold level as shown in this normalized linear scale depiction. LP-log-linear phase of signal generated during the exponential part of the PCR amplification; TP-a slowing of the amplification and accompanying fluorescence signal marks the transition phase; PP-the plateau phase is reached when there is little or no increase in fluorescent signal despite continued cycling.