


Dec 13, 2024

Version 2

Mouse Perfusion Protocol V.2

DOI

<https://dx.doi.org/10.17504/protocols.io.4r3l29qr3v1y/v2>



Heath Robinson¹

¹Cornell University



Heath Robinson

Cornell University

Create & collaborate more with a free account

Edit and publish protocols, collaborate in communities, share insights through comments, and track progress with run records.

Create free account

OPEN  ACCESS



DOI: <https://dx.doi.org/10.17504/protocols.io.4r3l29qr3v1y/v2>

Protocol Citation: Heath Robinson 2024. Mouse Perfusion Protocol. **protocols.io**

<https://dx.doi.org/10.17504/protocols.io.4r3l29qr3v1y/v2> Version created by **Heath Robinson**

License: This is an open access protocol distributed under the terms of the **Creative Commons Attribution License**, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited

Protocol status: Working

We use this protocol and it's working

Created: December 13, 2024

Last Modified: December 13, 2024

Protocol Integer ID: 115533

Keywords: Perfusion, mouse perfusion protocol protocol, perfusing mice, mice, protocol

Funders Acknowledgements:

Heath Robinson

Grant ID: F32MH134673

Disclaimer

DISCLAIMER – FOR INFORMATIONAL PURPOSES ONLY; USE AT YOUR OWN RISK

The protocol content here is for informational purposes only and does not constitute legal, medical, clinical, or safety advice, or otherwise; content added to protocols.io is not peer reviewed and may not have undergone a formal approval of any kind. Information presented in this protocol should not substitute for independent professional judgment, advice, diagnosis, or treatment. Any action you take or refrain from taking using or relying upon the information presented here is strictly at your own risk. You agree that neither the Company nor any of the authors, contributors, administrators, or anyone else associated with protocols.io, can be held responsible for your use of the information contained in or linked to this protocol or any of our Sites/Apps and Services.


Abstract

Protocol for perfusing mice with fixative, including description of creating all required solutions.

Materials

Equipment:

Surgical Platform

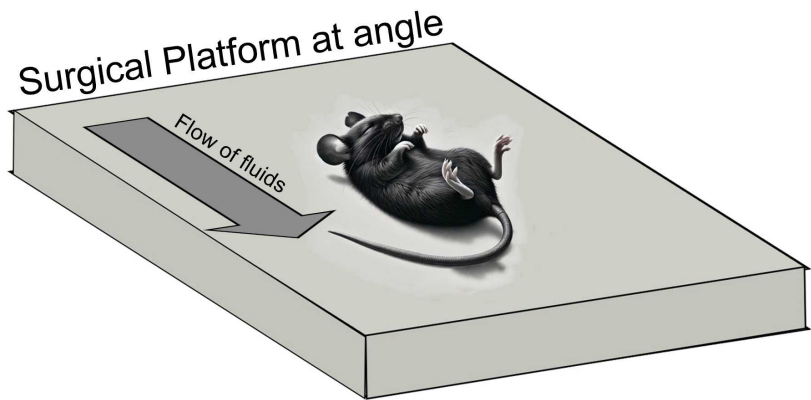

Surgical platform at an angle that allows for flow of fluids off platform waste disposal.

Equipment

Surflo winged infusion set 21G 3/4

NAME

Terumo

BRAND

TER 3SV-21BLK

SKU

Equipment

Insulin gauge needle (BD Ultra-fine™ II, NJ, USA)

NAME

(8 mm x 0.3 mm)

TYPE

BD

BRAND

328838

SKU

<https://www.bd.com/en-sg/offerings/diabetes-care/insulin-syringes/bd-insulin-syringes-with-bd-ultra-fine-needle-8mm-x30g>

LINK

0.3 mL

SPECIFICATIONS

Equipment

Variable-Flow Peristaltic Pump

NAME

Fisherbrand

BRAND

13-876-2

SKU

<https://www.fishersci.com/shop/products/fisher-scientific-variable-flow-peristaltic-pumps-4/p-158215>

LINK

Reagents:

☒ PBS Tablets, Phosphate Buffered Saline, Fisher BioReagents **Fisher Scientific Catalog #BP2944100**

☒ Paraformaldehyde Powder (PFA) **Catalog #P6148**

☒ Sodium Hydroxide **Fisher Scientific Catalog #BP359500**

1000ml of 4% PFA solution preparation:

1. Measure  600 mL of ddH₂O in

a graduated cylinder, and heat it to  70 °C to  90 °C (note: not directly heating with

- buffer).
2. Weigh  40 g of  Paraformaldehyde Powder (PFA) **Catalog #P6148** , and dissolve it in the above-mentioned solution that is continuously heated, stir, and add an appropriate amount of NaOH (about  0.1 g for  1000 mL) to aid the PFA dissolving.
 3. Add 10 tablets of  PBS Tablets, Phosphate Buffered Saline, Fisher BioReagents **Fisher Scientific Catalog #BP2944100**
 4. Make the volume to  1000 mL .
 5. Adjust the PH value to  7.2 -  7.4 (<  0.3 g  Sodium Hydroxide **Fisher Scientific Catalog #BP359500** , need not adjust the PH).
 6. Filter with

Equipment

Millipore® Stericup® Quick Release Vacuum Filtration System NAME

0.22 um polyethersulfone membrane filtration system TYPE

Millipore BRAND

All Photos(3) Key Documents COA/COQ View All Docum SKU

<https://www.sigmaaldrich.com/US/en/product/mm/s2gpu05re> LINK

0.22 um filter SPECIFICATIONS



7. Bottle and store at  4 °C until use.



Safety warnings

- ❗ Paraformaldehyde (PFA) and sodium hydroxide are hazardous substances that can be dangerous if not handled safely. Waste includes previous hazardous chemicals, as well as potential biological hazards. Handling should only be done with proper personal protection

Ethics statement

Experiments involving animals must be conducted according to internationally accepted standards. Users should always have prior approval from an Institutional Animal Care and Use Committee (IACUC) or equivalent ethics committee(s). Prior ethics approval should be obtained before performing these experiments.

Before start

Ensure the animal is under proper anesthesia plane per local University and IACUC standards.

Perfusion Steps

- 1 Rinse the peristaltic pump thoroughly with saline or PBS for more than 5 minutes
- 2 Start the peristaltic pump with normal saline/PBS, make sure everything is well connected (pump, tube, needles, saline/PFA), and there are no air bubbles in the tube.
- 3 After anesthesia, the animals are fixed tightly with pins on four paws. Open the abdominal and thoracic cavity with forceps in the left hand and scissors in the right hand. Remember that the tips of scissors are as close as possible to the bone to reduce the possibility of cutting the blood vessels.


Safety information

Anesthesia for euthanasia must follow and abide by local IACUC and University standards. Ensure proper anesthesia plane before performing perfusion.

- 4 Cut a small hole in the right atrium, inject saline with a needle connected to a tube in the pump into the left ventricular, and you will find blood flowing out of the right atrium.

Note

The angle of injection should be 45 degrees towards the Aortic Arch

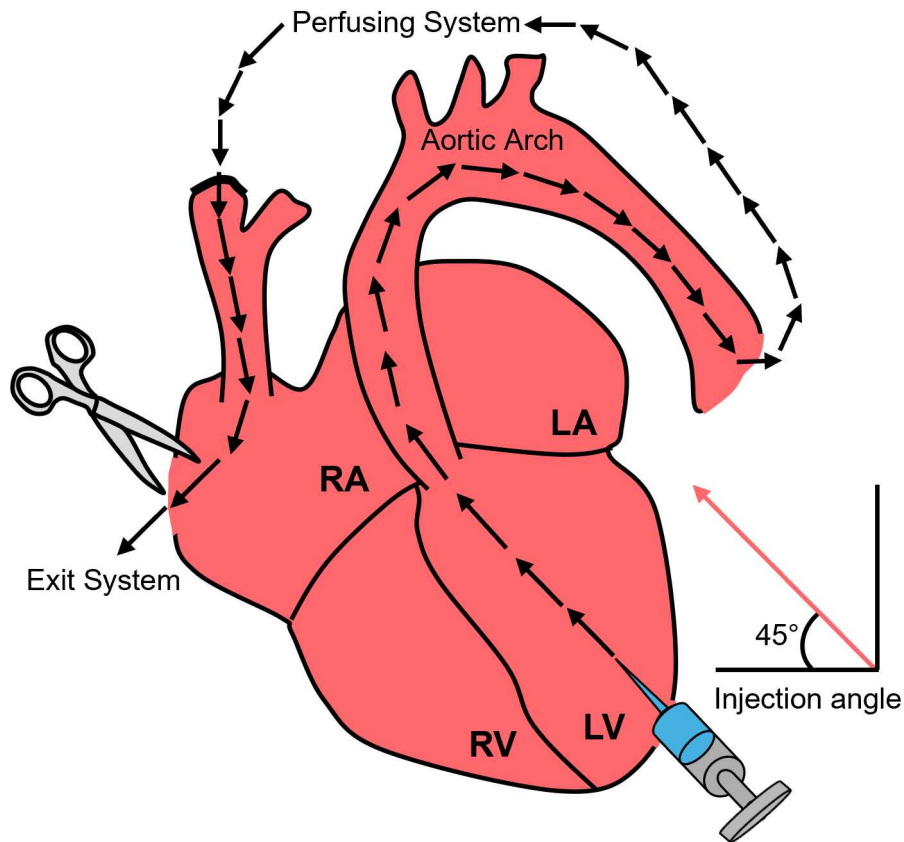

- 5 Perfuse with PBS for less than 5 minutes and stop the pump when the saline running out of the right atrium is clear (no blood is found). Change the tube from a saline bottle to a 4% PFA bottle (stop the pump first and change the tube second to reduce the possibility of bubbles in the tube). Open the pump again and perfuse animals with 4% PFA for another 10 minutes.

Note

Optimal flow settings for listed Peristaltic Pump (below) is between 32-25.

Equipment

Variable-Flow Peristaltic Pump

NAME

Fisherbrand

BRAND

13-876-2

SKU

<https://www.fishersci.com/shop/products/fisher-scientific-variable-flow-peristaltic-pumps-4/p-158215>

LINK

Note

Proper perfusion will result in tail rising upwards upon PFA perfusion.

Safety information

Paraformaldehyde (PFA) is a hazardous substance that can be dangerous if not handled safely

5.1 10 minutes for adults and 7 minutes for younger than P10.

6 Dissect the brain, and keep the tips of scissors as close as possible to the bone. This will reduce the damage to the brain tissue. Post fixed tissues in 4% PFA for less than 1 hour or in PFA overnight.

Safety information

Dispose of waste in accordance with local EHS standards.

