



Oct 10, 2022

Version 2

PCR cleanup and size selection with magnetic beads V.2

 In 4 collections

DOI

<https://dx.doi.org/10.17504/protocols.io.36wgqj45xvk5/v2>



Dominik Buchner¹

¹University of Duisburg-Essen, Aquatic Ecosystem Research



Dominik Buchner

University of Duisburg-Essen, Aquatic Ecosystem Research

Create & collaborate more with a free account

Edit and publish protocols, collaborate in communities, share insights through comments, and track progress with run records.

Create free account

OPEN  ACCESS



DOI: <https://dx.doi.org/10.17504/protocols.io.36wgqj45xvk5/v2>

Protocol Citation: Dominik Buchner 2022. PCR cleanup and size selection with magnetic beads. **protocols.io** <https://dx.doi.org/10.17504/protocols.io.36wgqj45xvk5/v2> Version created by **Dominik Buchner**

License: This is an open access protocol distributed under the terms of the **Creative Commons Attribution License**, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited



Protocol status: Working

We use this protocol and it's working

Created: October 10, 2022

Last Modified: October 10, 2022

Protocol Integer ID: 71082

Keywords: pcr cleanup, carboxylated beads, magnetic beads, PEG-NaCl precipitation, size selection, buffer exchange, pcr cleanup, pcr product, pcr, size selection with magnetic bead, magnetic bead, dna extract, nacl buffer, dna, bead, buffer exchange

Abstract

This protocol describes how to clean up PCR products or DNA extracts and perform a size selection with carboxylated-magnetic beads and a PEG-NaCl buffer. It can also be used for volume reduction of a sample or for buffer exchange.

Guidelines


Follow general lab etiquette. Wear gloves to prevent contaminating the samples. Clean the workspace before starting with 80% EtOH.

Ratio Guide:


To get an estimate the performance of different ratios the protocol was tested using a DNA Ladder

 GeneRuler 100 bp DNA Ladder ready-to-use **Thermo Fisher Scientific Catalog #SM0243**. The eluate was then measured using a Fragment Analyzer with the High Sensitivity Kit.


Input DNA:

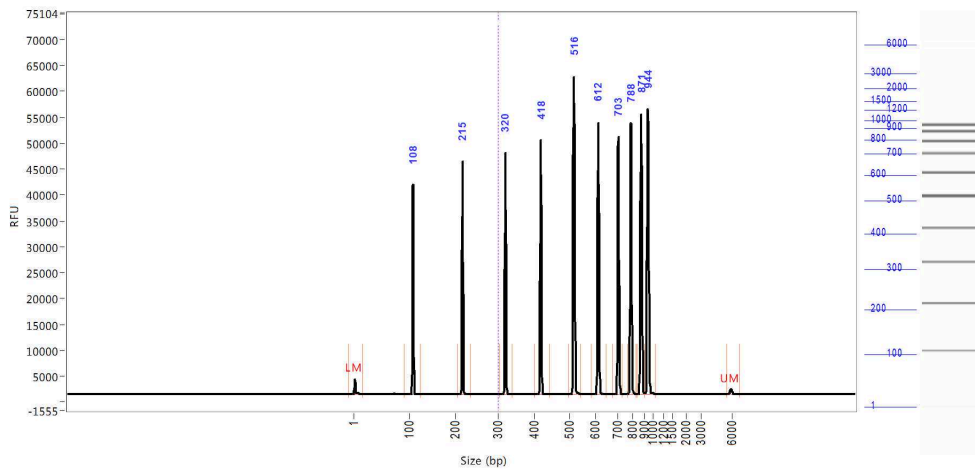


Ratio 1.8:

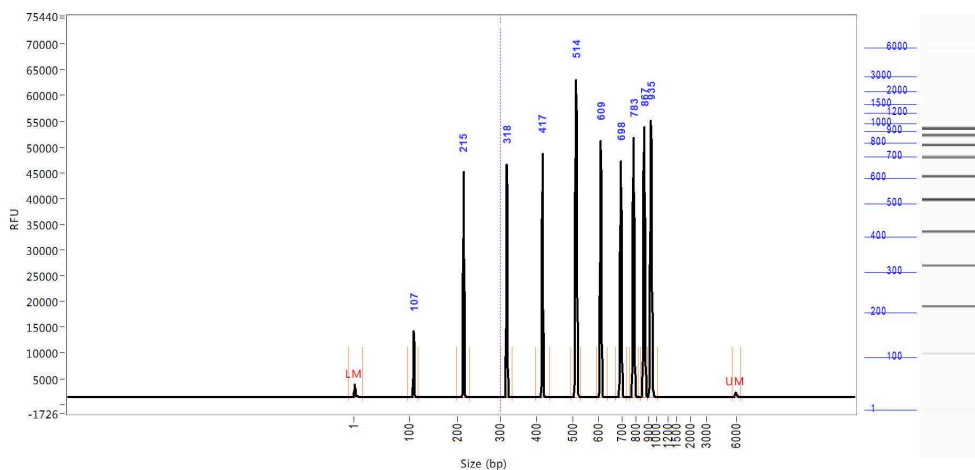


Ratio 1:

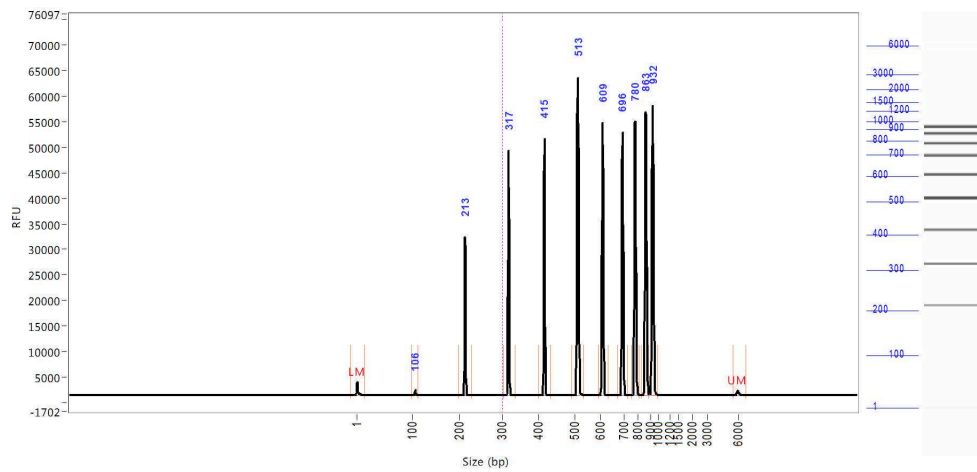


Ratio 0.9:

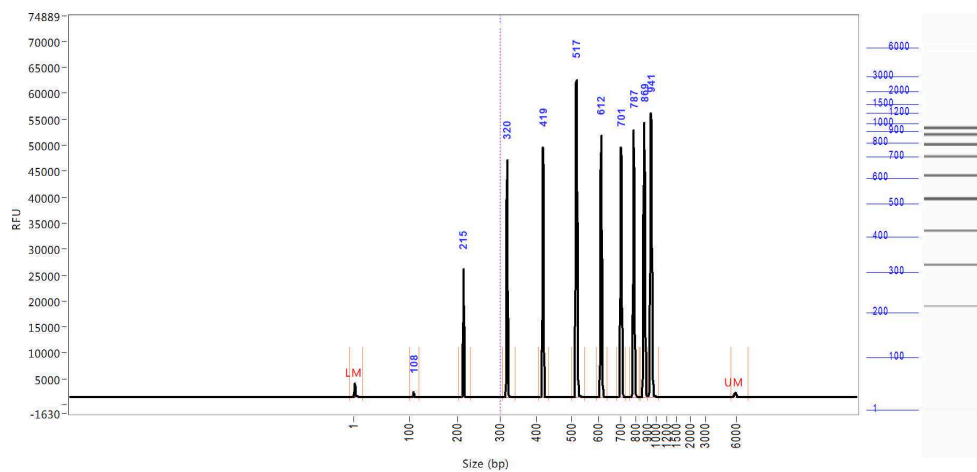


Ratio 0.85:

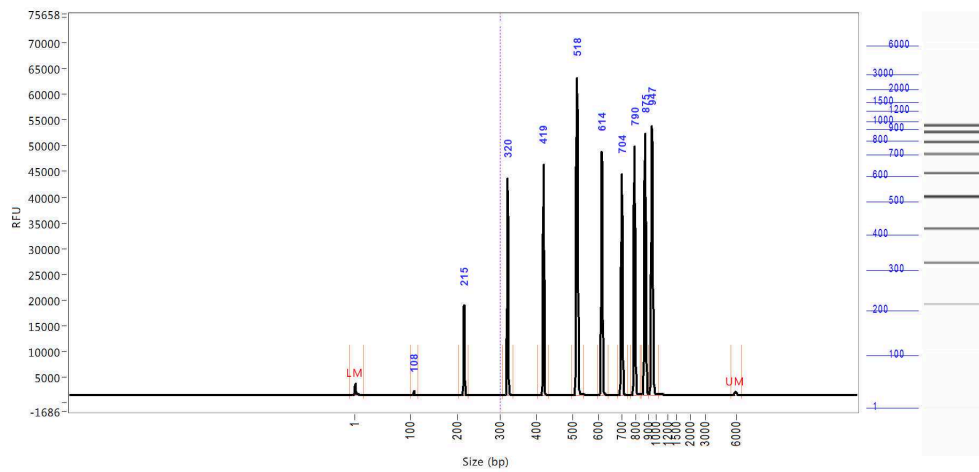


Ratio 0.8:

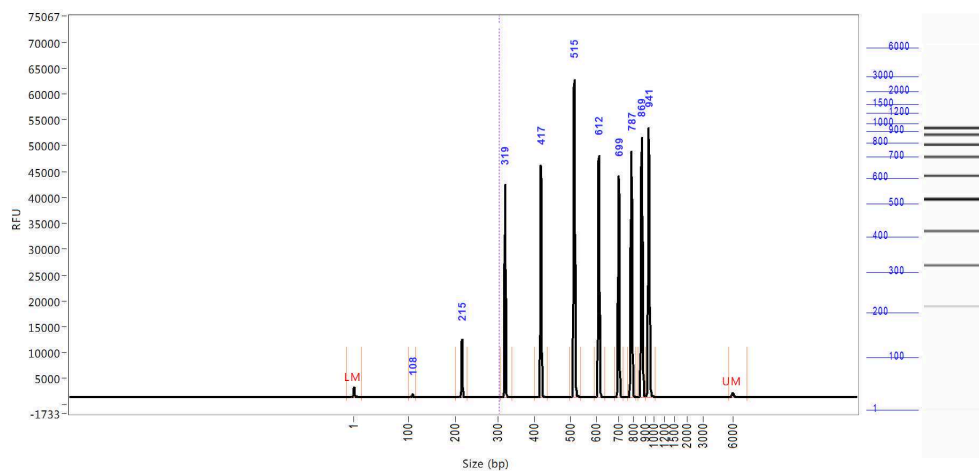


Ratio 0.75:

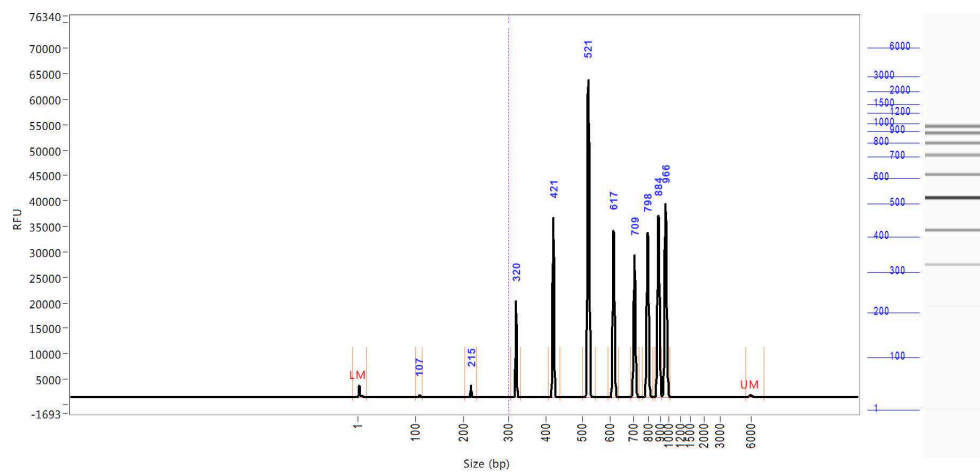


Ratio 0.7:

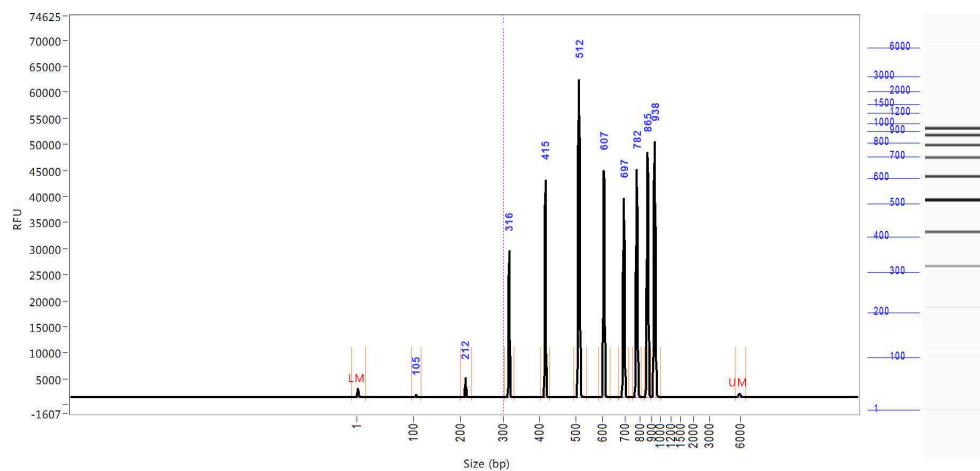


Ratio 0.65:

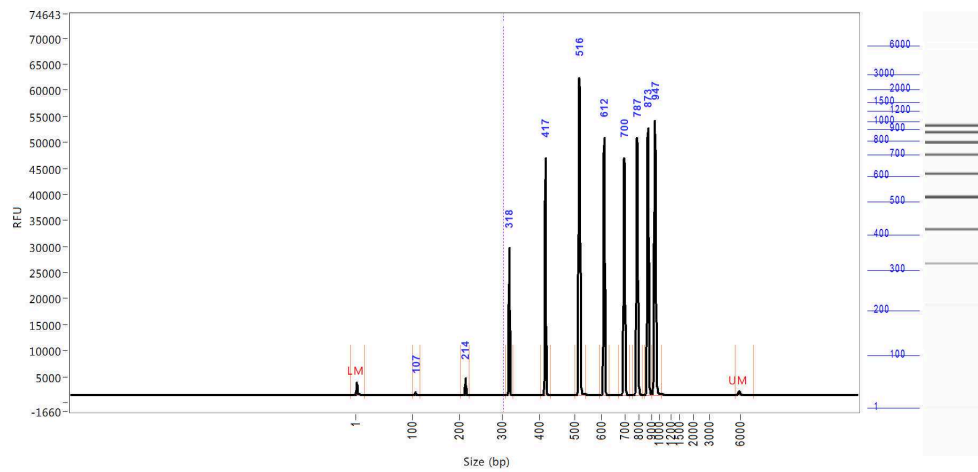

Ratio 0.6:

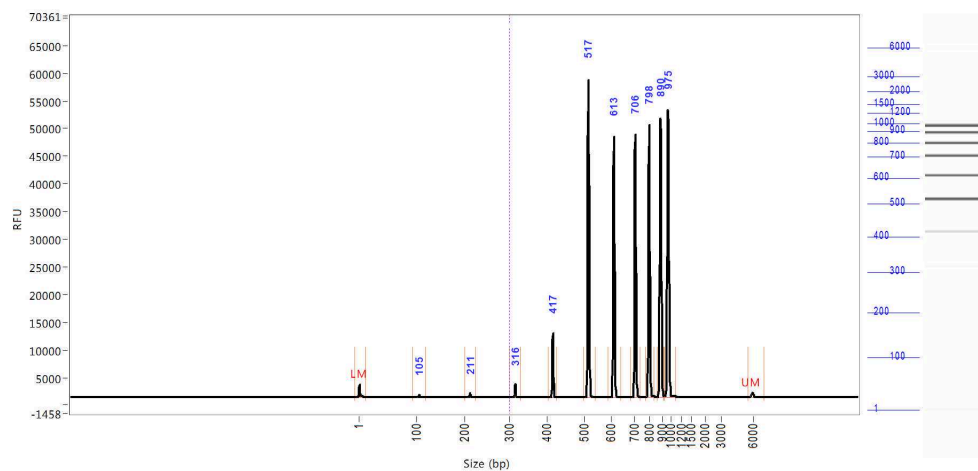

Ratio 0.55:

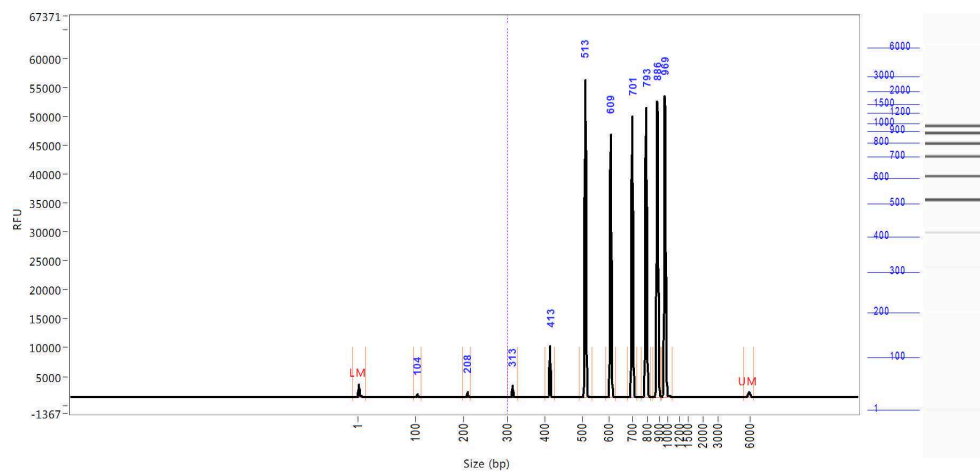

Materials

Materials required:

Below all materials needed for the protocol are listed. Vendors and part numbers are listed but interchangeable depending on the supply situation.

Chemicals:

Ethanol absolute  Ethanol absolute 99.8% **Fisher Scientific Catalog #11994041**

Hydrochloric acid fuming 37%

 Hydrochloric acid fuming 37% **Merck MilliporeSigma (Sigma-Aldrich) Catalog #1003171011**

Tris ultrapure 99.9%  Tris ultrapure 99.9% **Diagonal Catalog #A1086.1000**

EDTA disodium salt  EDTA disodium salt **Merck MilliporeSigma (Sigma-Aldrich) Catalog #E5134-50G**

Tween 20  Tween 20 **Carl Roth Catalog #9127.1**

Sera-Mag SpeedBeads

 Sera-Mag SpeedBeads carboxylate modified particles **Merck MilliporeSigma (Sigma-Aldrich) Catalog #GE45152105050350**

PCR-grade water

 Invitrogen UltraPure DNase/RNase-Free Distilled Water **Fisher Scientific Catalog #11538646**

Labware:

125 mL Nalgene Wide-Mouth Bottle

 Thermo Scientific Nalgene Wide-Mouth LDPE Bottle with Closure **Fisher Scientific Catalog #10044180**

Large magnet  Neodyme magnet **Magnethandel Catalog #3935**

96-well plate magnet  MM-Seperator M96 **Carl Roth Catalog #2141.1**

Hard-Shell PCR Plate  Hard-Shell 96-well PCR plate **Bio-Rad Laboratories Catalog #HSP9601**

Clear Polystyrene 96-Well Microplate

 Corning Clear Polystyrene 96-Well EIA/RIA Microplate **Fisher Scientific Catalog #10380982**

Stock solutions:

 1 L Tris stock solution  1 Mass Percent  8.5

- Add  121.14 g Tris ultrapure 99.9% to a beaker
- Adjust volume to  800 mL with ddH₂O
- Adjust pH to  8.5 with HCl



- Adjust volume to 1 L with ddH₂O
- Sterilize by filtering and store at Room temperature

1 L Tris stock solution 1 Mass Percent 8

- Add 121.14 g Tris ultrapure 99.9% to a beaker
- Adjust volume to 800 mL with ddH₂O
- Adjust pH to 8 with HCl
- Adjust volume to 1 L with ddH₂O
- Sterilize by filtering and store at Room temperature

1 L Tris stock solution 1 Mass Percent 7.5

- Add 121.14 g Tris ultrapure 99.9% to a beaker
- Adjust volume to 800 mL with ddH₂O
- Adjust pH to 7.5 with HCl
- Adjust volume to 1 L with ddH₂O
- Sterilize by filtering and store at Room temperature

1 L EDTA stock solution 0.5 Mass Percent 8

- Add 186.12 g EDTA disodium salt to a beaker
- Adjust volume to 1 L with ddH₂O
- Adjust pH to 8 with sodium hydroxide
- Sterilize by filtering and store at Room temperature

1 L wash buffer stock solution (50 millimolar (mM) Tris) 7.5

- Add 50 mL Tris stock solution 7.5 to a beaker
- Adjust volume to 1 L with ddH₂O
- Sterilize by filtering and store at Room temperature

1 L PEG-NaCl buffer (2.5 Mass Percent NaCl , 20 Mass / % volume PEG 8000 , 10 millimolar (mM) Tris , 1 millimolar (mM) EDTA , 0.05 % (v/v) Tween 20) 8

- Add 200 g NaCl to a beaker
- Add 146.2 g PEG 8000

- Add 10 mL Tris stock solution pH 8
- Add 2 mL EDTA stock solution pH 8
- Add 250 µL of Tween 20
- Adjust volume to 1 L with ddH₂O
- Dissolve the PEG and NaCl by stirring and heating to 80 °C the solution will become milky at this point.
- Let the solution cool down to Room temperature
- Sterilize by filtering and store at 4 °C

Working solutions:

1 L TE minimum buffer (10 millimolar (mM) Tris , 1 millimolar (mM) EDTA) pH 8

- Add 10 mL Tris stock solution pH 8 to a beaker
- Add 200 µL EDTA stock solution pH 8
- Adjust volume to 1 L with ddH₂O
- Sterilize by filtering and store at Room temperature

1 L wash buffer (10 millimolar (mM) Tris , 80 % (v/v) Ethanol) pH 7.5

- Add 200 mL wash buffer stock solution
- Adjust volume to 1 L with Ethanol absolute
- Sterilize by filtering and store at Room temperature

1 L elution buffer (10 millimolar (mM) Tris) pH 8.5

- Add 10 mL Tris stock solution pH 8.5 to a beaker
- Adjust volume to 1 L with ddH₂O
- Sterilize by filtering and store at Room temperature

100 mL cleanup solution pH 8

- Add 2 mL Sera-Mag SpeedBeads carboxylate modified to a clean 125 mL Nalgene bottle
- Add 25 mL TE minimum buffer
- Shake the bottle to wash the beads
- Place the bottle on a large magnet for 00:05:00 to pellet the beads
- Discard the supernatant
- Add 25 mL TE minimum buffer



- Shake the bottle to wash the beads
- Place the bottle on a large magnet for 00:05:00 to pellet the beads
- Discard the supernatant
- Add 100 mL PEG-NaCl buffer
- Shake well to resuspend the beads
- Store at 4 °C

Safety warnings

Reagents are potentially damaging to the environment. Dispose waste responsibly.

Before start

Make sure all buffers are prepared before starting.

For easier pipetting let the bead-solution adjust to Room temperature

Note

The protocol described here is designed for the use of 250 μ L U-bottom assay plates but can also be done in tubes, PCR plates, strips, or any sufficient reaction vessel. The recommended shaking speeds are adjusted to the plates mentioned in the materials.



- 1 Shake the **cleanup solution** until the beads are homogeneously resuspended

Note

The protocol described here uses a **cleanup solution** to **sample** ratio of 0.8:1. This is sufficient for the removal of primer and primer dimers below a size of 200 bp. For the removal of shorter or larger fragments, the ratio has to be adjusted accordingly. For more information on ratios refer to the material provided in the tab "Guidelines".

- 2 Add  30 µL PCR-grade water and  32 µL of cleanup solution to a  250 µL U-bottom assay plate

Note

It's recommended to increase the volume of the sample with PCR-grade water for easier liquid handling but also to lower relative pipetting error (e.g. if the pipette is off by  2 µL the effect on the ratio is larger if working with a  10 µL assay than when working with a  80 µL assay.

The amount of beads is calculated as follows:
(sample volume + water volume) * ratio = cleanup solution volume

In this example:

( 10 µL PCR product +  30 µL PCR-grade water) * 0.8 =
 32 µL cleanup solution

For higher sample numbers PCR-grade water and cleanup solution can be prepared as a master mix.

- 3 Add  10 µL of sample.

Note

This protocol works for the cleanup of PCR products as well as the cleanup of DNA extracts or for buffer exchange after enzyme treatment of samples.

- 4



To bind the DNA to the beads shake at  900 rpm, Room temperature , 00:05:00

Note

If the protocol is not done in plates mixing can also be accomplished by pipetting or vortexing.

5 Place the plate on a magnet to pellet the beads for  00:02:00

2m

Note

Depending on the magnet and volume used separation times may vary and have to be adjusted accordingly.

6 Discard the supernatant by pipetting

7 With the plate still on the magnet, add  100 μ L of wash buffer to each sample

8 Incubate for at least  00:00:30

30s

9 Discard the supernatant by pipetting

10  and repeat once for a total of 2 washes

11 With the plate still on the magnet, incubate the plate for  00:05:00 at  Room temperature to dry off residuals of wash buffer

5m

12 Add  40 μ L of elution buffer to each sample



13  900 rpm, Room temperature , 00:05:00 to elute the DNA from the beads

14 Place the plate on a magnet to pellet the beads for  00:02:00

2m

15 Transfer  30 μ L of the DNA to a new PCR plate. Store at  -20 °C

Note

Leaving  10 μ L of elution buffer is recommended to avoid carry-over of beads. If all of the DNA is needed for subsequent analysis try to pipette slowly without disturbing the pellet.