

Aug 12, 2018

Version 3

Primer ID MiSeq Library Prep V.3

DOI


<https://dx.doi.org/10.17504/protocols.io.sjdec6>

Shuntai Zhou¹

¹University of North Carolina at Chapel Hill



Shuntai Zhou



Create & collaborate more with a free account

Edit and publish protocols, collaborate in communities, share insights through comments, and track progress with run records.

Create free account

OPEN  ACCESS



DOI: <https://dx.doi.org/10.17504/protocols.io.sjdec6>

Protocol Citation: Shuntai Zhou 2018. Primer ID MiSeq Library Prep. **protocols.io**
<https://dx.doi.org/10.17504/protocols.io.sjdec6>

License: This is an open access protocol distributed under the terms of the **Creative Commons Attribution License**, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited

Protocol status: Working

We use this protocol and it's working

Created: August 11, 2018

Last Modified: August 12, 2018

Protocol Integer ID: 14661

Keywords: NGS, Primer ID, qiaamp viral rna extraction kit, primer id miseq library prep, viral rna extraction kit, cdna primer, primer id miseq, viral rna, sequencing library, rna extraction, cdna synthesis, primer id, kapa hifi pcr kit, rna, random nucleotide, pcr, using qiaamp, primer, cdna, block of random nucleotide, nucleotide, rounds of pcr

Abstract

This is the protocol to prepare Primer ID MiSeq sequencing library. Viral RNA was first extracted using QIAamp viral RNA extraction kit. The block of random nucleotides (Ns) in the cDNA primers served as the Primer ID. The Superscript III kit was used for the cDNA synthesis. We used two rounds of PCR to amplify the cDNA and incorporate Illumina indexed adapters with KAPA2G Robust and KAPA HiFi PCR kits, respectively.

Attachments




[amplicon protocol_v1...](#)

222KB

Guidelines

Viral RNA extraction using QIAamp vRNA mini kit.

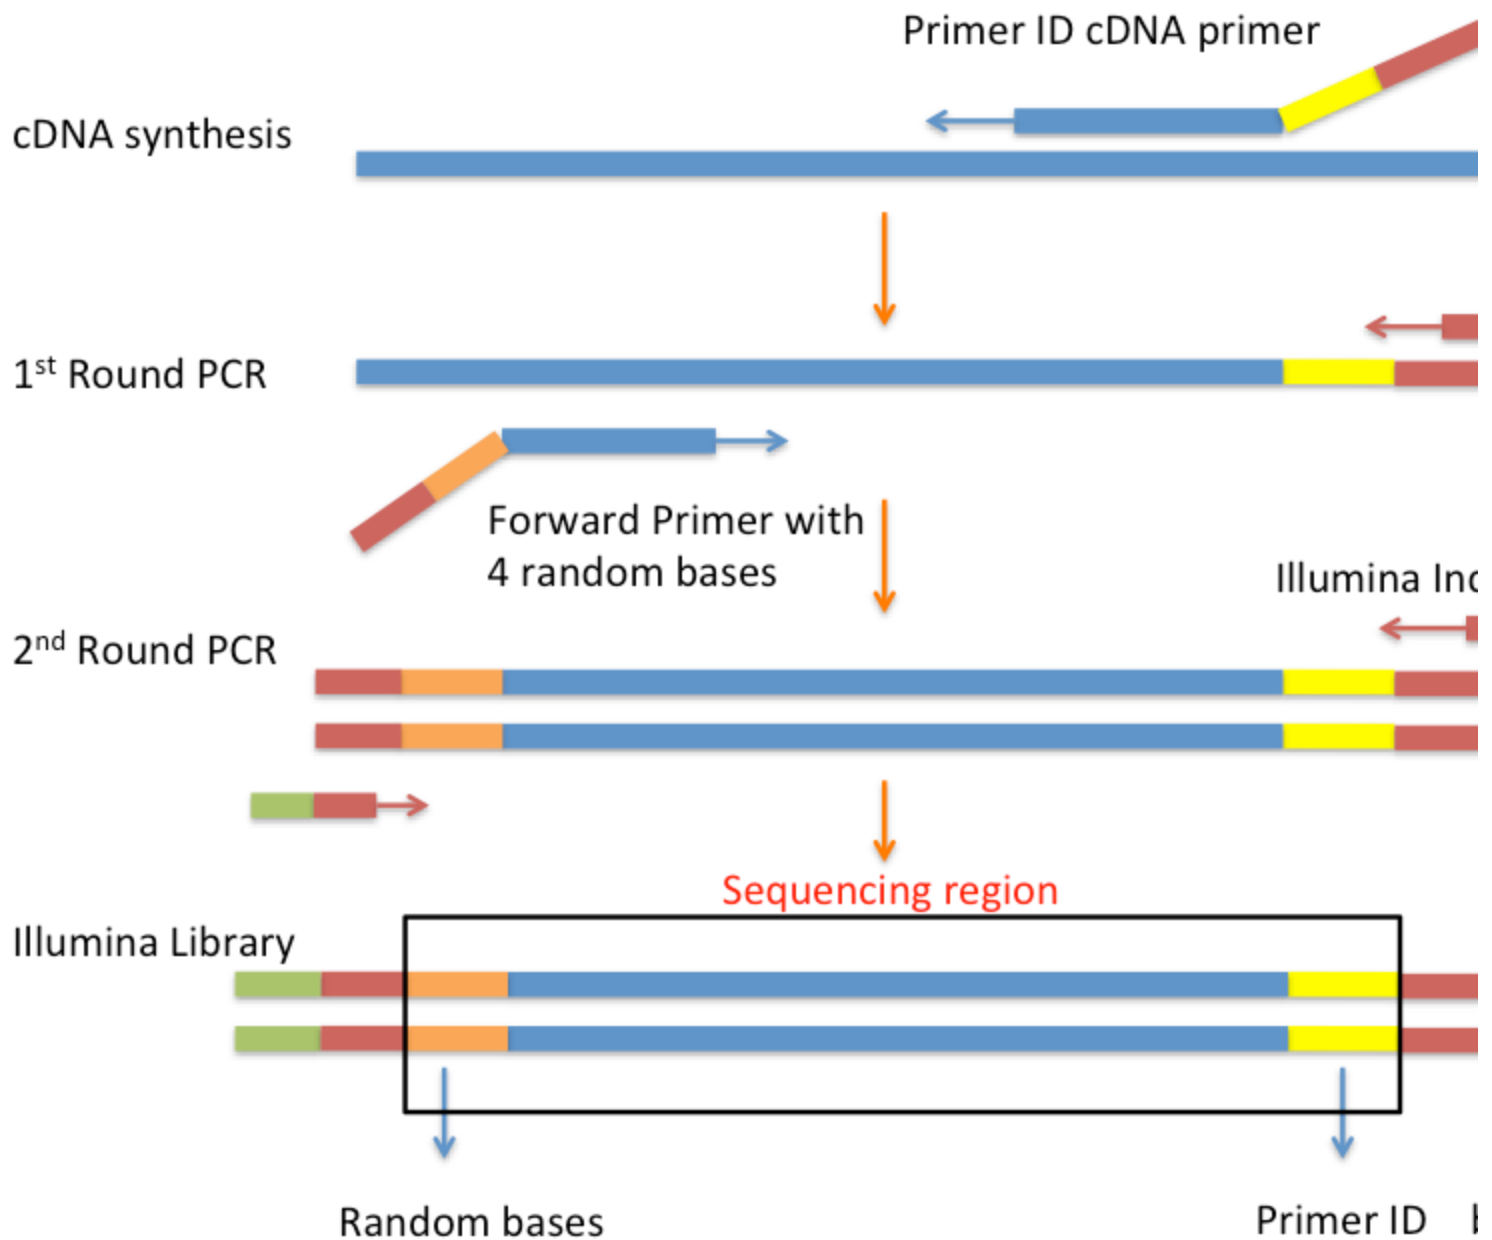

Primers (NOTE: HIV-1 ENV REGION AS AN EXAMPLE, SUBSTITUTE 1 in the forward primer and cDNA primer)

V1F(forward) 5'-3'	GCCTCCCTCGCGCCATCAGAGATGTGTATAAGAGACAG AAAGCCTAAAGCCATGTGTA
BV3R Uni (cDNA Primer) 5'-3'	GTGACTGGAGTTCAGACGTGTGCTCTTCCGATCTNNNN TGCTCTACTAATGTTACAATGTGC
Universal Adapter	AATGATACGGCGACCACCGAGATCTACACGCCTCCCTC G
Indexed Adapter	CAAGCAGAAGACGGCATACGAGATNNNNNNGTGACT GCTC
ADPT_2a	GTGACTGGAGTTCAGACGTGTGCTC

Note: Primer ID primer and forward primer use random bases. Indexed primers have 24 fixed barcodes.

Table of Indexed Primers

Indexed Primer	Index	Index Sequence	Sequence
PCR Primer, Index 1	1	ATCACGA	CAAGCAGAAGACGGCATAACGAGAT CGTGAT GTG
PCR Primer, Index 2	2	CGATGTA	CAAGCAGAAGACGGCATAACGAGAT ACATCG GTG
PCR Primer, Index 3	3	TTAGGCA	CAAGCAGAAGACGGCATAACGAGAT GCCTAA GTG
PCR Primer, Index 4	4	TGACCAA	CAAGCAGAAGACGGCATAACGAGAT TGGTCA GTG
PCR Primer, Index 5	5	ACAGTGA	CAAGCAGAAGACGGCATAACGAGAT CACTGT GTG
PCR Primer, Index 6	6	GCCAATA	CAAGCAGAAGACGGCATAACGAGAT ATTGGC GTG
PCR Primer, Index 7	7	CAGATCA	CAAGCAGAAGACGGCATAACGAGAT GATCTG GTG
PCR Primer, Index 8	8	ACTTGAA	CAAGCAGAAGACGGCATAACGAGAT TCAAGT GTG
PCR Primer, Index 9	9	GATCAGA	CAAGCAGAAGACGGCATAACGAGAT CTGATC GTG
PCR Primer, Index 10	10	TAGCTTA	CAAGCAGAAGACGGCATAACGAGAT AAGCTA GTG
PCR Primer, Index 11	11	GGCTACA	CAAGCAGAAGACGGCATAACGAGAT GTAGCC GTG
PCR Primer, Index 12	12	CTTGTA	CAAGCAGAAGACGGCATAACGAGAT TACAAG GTG
PCR Primer, Index 13	13	TCCATAA	CAAGCAGAAGACGGCATAACGAGAT TATGGA GTG
PCR Primer, Index 14	14	GTACTAA	CAAGCAGAAGACGGCATAACGAGAT TAGTAC GTG
PCR Primer, Index 15	15	ACAGTAA	CAAGCAGAAGACGGCATAACGAGAT TACTGT GTG
PCR Primer, Index 16	16	CTCATGA	CAAGCAGAAGACGGCATAACGAGAT CATGAG GTG
PCR Primer, Index 17	17	ACGATAA	CAAGCAGAAGACGGCATAACGAGAT TATCGT GTG
PCR Primer, Index 18	18	TGCAGAA	CAAGCAGAAGACGGCATAACGAGAT TCTGCA GTG
PCR Primer, Index 19	19	TTCATAA	CAAGCAGAAGACGGCATAACGAGAT TATGAA GTG
PCR Primer, Index 20	20	TGCTGTA	CAAGCAGAAGACGGCATAACGAGAT ACAGCA GTG
PCR Primer, Index 21	21	TATCACA	CAAGCAGAAGACGGCATAACGAGAT GTGATA GTG
PCR Primer, Index 22	22	TGGATAA	CAAGCAGAAGACGGCATAACGAGAT TATCCA GTG
PCR Primer, Index 23	23	CGCATTA	CAAGCAGAAGACGGCATAACGAGAT AATGCG GTG
PCR Primer, Index 24	24	GCCTTAA	CAAGCAGAAGACGGCATAACGAGAT TAAGGC GTG

Materials

MATERIALS

☒ QIAamp vRNA mini kit Qiagen Catalog #51304

☒ Agencourt RNAClean XP Beckman Coulter Catalog #A63987

☒ 70% ethanol

☒ DNase-free water

☒ AmpureXP PCR cleanup kits Beckman Coulter Catalog #A63880

☒ QIAquick gel extraction kit Qiagen Catalog #28704

☒ Qubit dsDNA BR Assay kit Invitrogen - Thermo Fisher Catalog #Q32850

Prepare Primer Mix (Optional, only for multiplexed Primer ID library prep)

1 For multiplexing sequencing, first, prepare Primer Mix.

Example (For HIV drug resistance pipeline).

Regions	DR cDNA primer	DR F primer
PR	R2614_PID	F2163AD
RT	R3284_PID11	F2620_AD
INT	R4752_PID11	F4383_AD
V3	V3R_Buni_11	V1F_AD

Make 10 μ M primer mix: mix 10 μ L of each primer in one set and 60 μ L of dH₂O.

Primer Tables

primer	sequence (5'-3')
R2614_P ID	GTGACTGGAGTTCAGACGTGTGCTCTTCCGATCTNNNNNNNNNNCAGTTT AACTTTTGGGCCATCCATTCC
R3284_PID11	GTGACTGGAGTTCAGACGTGTGCTCTTCCGATCTNNNNNNNNNNCAGT CACTATAGGCTGTACTGTCCATTTATC
R4752_PID11	GTGACTGGAGTTCAGACGTGTGCTCTTCCGATCTNNNNNNNNNNNATCG AATACTGCCATTTGTACTGC
R7209_PID11	GTGACTGGAGTTCAGACGTGTGCTCTTCCGATCTNNNNNNNNNNNCAGT CCATTTTGCTYTAYTRABVTTACAATRTGC
F2163A D	GCCTCCCTCGCGCCATCAGAGATGTGTATAAGAGACAGNNNNTCAGAGC AGACCAGAGCCAACAGCCCCA
F2620_AD	GCCTCCCTCGCGCCATCAGAGATGTGTATAAGAGACAGNNNNGGCCATT GACAGAAGAAAAAATAAAAGC
F4383_AD	GCCTCCCTCGCGCCATCAGAGATGTGTATAAGAGACAGNNNNAAAAGGA GAAGCCATGCATG
V1F_AD	GCCTCCCTCGCGCCATCAGAGATGTGTATAAGAGACAGNNNNTTATGGG ATCAAAGCCTAAAGCCATGTGTA

"N" in this Primer table is a random nucleotide.

P1	AATGATACGGCGACCACCGAGATCTACACGCCTCCCTCGCGCCATC AGAGATGTG
----	---



Indexed Adapter	CAAGCAGAAGACGGCATACGAGAT NNNNNN GTGACTGGAGTTCAGACGTGTGCTC
ADPT_2a	GTGACTGGAGTTCAGACGTGTGCTC

The 6 "N"s are not random nucleotides. They are a set of 24 pre-designed indexed sequences.

- Mix well.

cDNA synthesis

- Pipette the following components into a 0.5 ml RNase-free tube:

	μl/tube		[stock]	[final]	[mastermix]
	3.0	dNTP Mix	10 mM each	0.5	
	1.5	cDNA primer	10 μM	0.25 μM	
	34.5	RNA template			
	39.00	Total volume			

🧪 3 μL dNTPMix

🧪 1.5 μL cDNA primer

🧪 34.5 μL RNA template

- Place tube in 65°C heat block for 3-5'.

🕒 00:05:00 65°C heat block

- Place the tube on ice for 1'.

🕒 00:01:00 on ice

- Add the following components:

	μl/tube		[stock]	[final]	[mastermix]
	12.0	5x buffer	5x	1x	
	3.0	DTT	100 mM	5	
	3.0	RNaseOUT	40 u/μl	2	
	3.0	SSIII RT	200 u/μl	10	



	21.0	Per tube			
--	------	----------	--	--	--

 12 µL 5x buffer

 3 µL DTT

 3 µL RNaseOUT

 3 µL SSII RT

7 Mix and incubate at 50°C for 1 hr.

 01:00:00 Incubation at 50°C

8 Increase to 55°C and incubate for 1 hr.

 01:00:00 Incubation at 55°C

9 Inactivate SSIII RT by heating at 70°C for 15'.

 00:15:00 Heating at 70°C

10 To each tube, add 1 µL RNase H, incubate at 37°C for 20'.

 1 µL RNase H

 00:20:00 Incubation at 37°C

Purification

11 Purify cDNA using Agencourt RNAClean XP.
Resuspend the beads and take an aliquot out. Keep at room temperature for at least **30 minutes** before use. (Should be in 1ml aliquots)

 00:30:00 Room temperature

12 Transfer the cDNA reactions into 1.7 mL RNase-free tubes.

13 Resuspend the beads (Vortex). Add **42 µL of beads to 60 µL cDNA (Ratio: 0.6 – 0.8)** Agencourt RNAClean XP beads to each cDNA reaction.

 42 µL beads

 60 µL cDNA

14 Mix the Agencourt RNAClean XP and sample thoroughly by pipette mixing 15 times. No **vortexing**. Let the tube incubate at room temperature for **20 minutes** before proceeding to the next step.

 00:20:00 Room temperature



- 15 Place the tube onto the magnetic tube rack for **5 minutes** to separate the beads from solution.

00:05:00 Magnetic tube rack

- 16 Slowly aspirate the cleared solution from the tube and discard. This step should be performed while the tube is situated on the rack. Do not disturb the magnetic beads, which have formed a spot on the side of the tube.

- 17 Dispense 500 µL of 70% ethanol into the tube and incubate for **30 seconds** at room temperature. Aspirate out the ethanol and discard. (1/3)

It is important to perform this step with the tube situated **on the rack. Do not disturb the separated magnetic beads.** Be sure to remove all of the ethanol from the bottom of the well as it may contain residual contaminants.

00:00:30 Incubation at room temperature

- 18 Dispense 500 µL of 70% ethanol into the tube and incubate for **30 seconds** at room temperature. Aspirate out the ethanol and discard. (2/3)

It is important to perform this step with the tube situated **on the rack. Do not disturb the separated magnetic beads.** Be sure to remove all of the ethanol from the bottom of the well as it may contain residual contaminants.

00:00:30 Incubation at room temperature

- 19 Let the reaction tube air-dry **10 minutes** on the rack with the cap open. The tube(s) should air-dry until the last visible traces of ethanol evaporate. Over drying the sample may result in a lower recovery.

00:10:00 Air-drying

- 20 **(Optional for clinical samples)** Elute in 60 µl water. Repeat step 12 to 19.

[go to step #13](#) Optional for clinical samples

- 21 Remove the tube from the rack and resuspend beads in 24 µl DNase-free water by pipetting up and down. Place tube back on the rack and leave for **3 minutes**.

24 µL DNase-free water

00:03:00 Magnetic rack

- 22 Pipette the eluant from the tube while it is situated **on the magnetic tube rack.**

PCR 1

- 23 Complete thaw and vortex KAPA reagents (except for enzyme) before use.



24

	μl/tube		[stock]	[final]	[mastermix]
	10.0	5x Buffer A	5x	1x	
	10.0	Enhancer	5x	1x	
	1.0	dNTPs	10 mM	0.2 mM	
	2.5	Forward primer	10 μM	0.5 μM	
	2.5	ADPT_2a	10 μM	0.5 μM	
	0.5	KAPA Robust polymerase	5 U/μl	2.5 U	
	23.5	Template cDNA			

Prepare mastermix in cold box and use repeater pipette to add to each tube in the cold box. Add template cDNA to each tube and pipette up and down to mix.

🧪 10 μL 5x Buffer A

🧪 10 μL Enhancer

🧪 1 μL dNTPs

🧪 2.5 μL Forward primer

🧪 2.5 μL ADPT_2a

🧪 0.5 μL KAPA Robust polymerase

🧪 23.5 μL Template cDNA

25

Cycle

95°C	1 min
95°C	15 s
58°C	1 min
72°C	30 s
15-25 cycles	
72°C	3 min
4°C	On hold

Purification PCR products

- 26 Purify PCR products using AmpureXP PCR cleanup kits. Vortex the 1 ml aliquot and remove the needed volume. Keep at room temperature for at least **30 minutes** before use.
 00:30:00 Room temperature
- 27 Transfer the PCR1 reactions into 1.7 mL RNase-free tubes.
- 28 Resuspend the beads. Add **40 µl (Ratio: 0.6 – 0.8: 1, 36µl – 48µl)** Ampure XP beads to each cDNA reaction.
 40 µL Ampure XP beads
- 29 Mix the Ampure XP and sample thoroughly by **vortexing**. Let the tube incubate at room temperature for **5 minutes** before proceeding to the next step (incube off the rack).
 00:05:00 Incubation at room temperature
- 30 Place the tube onto the magnetic tube rack for **5 minutes** to separate the beads from solution.
 00:05:00 Incubation magnetic rack
- 31 Slowly aspirate the cleared solution from the tube and discard. This step should be performed while the tube is situated on the rack. Do not disturb the magnetic beads, which have formed a spot on the side of the tube.
- 32 Dispense 500 µL of 70% ethanol into the tube and incubate for **30 seconds** at room temperature. Aspirate out the ethanol and discard. (1/2)

Note

It is important to perform this step with the tube situated **on the rack**. **Do not disturb the separated magnetic beads**. Be sure to remove all of the ethanol from the bottom of the well as it may contain residual contaminants.

 500 µL 70% ethanol

 00:00:30 Incubation at room temperature

- 33 Dispense 500 µL of 70% ethanol into the tube and incubate for **30 seconds** at room temperature. Aspirate out the ethanol and discard. (2/2)

Note

It is important to perform this step with the tube situated **on the rack**. **Do not disturb the separated magnetic beads**. Be sure to remove all of the ethanol from the bottom of the well as it may contain residual contaminants.

🧪 500 µL 70% ethanol

⌚ 00:00:30 Incubation at room temperature

- 34 Let the reaction tube air-dry **10 minutes** on the rack with the cap open. The tube(s) should air-dry until the last visible traces of ethanol evaporate. Over drying the sample may result in a lower recovery.

⌚ 00:10:00 Air-drying

- 35 Remove the tube from the rack and resuspend beads in 50 µl DNase-free water by pipetting up and down. Place tube back on the rack and leave for **3 minutes**.

🧪 50 µL DNase-free water

⌚ 00:03:00 Magnetic rack

- 36 Pipette the 45 µl eluant from the tube while it is situated **on the magnetic tube rack**.

PCR 2

- 37 Complete thaw and vortex KAPA reagents (except for enzyme) before use.

38

µl/tube		[stock]	[final]	[mastermix]
5.0	5x KAPA HiFi Fidelity Buffer	5x	1x	
1.0	dNTP Mix	10 mM	0.4 mM	
1.0	Uni Adapter (ADPT_P1)	10 µM	0.4 µM	
0.5	KAPA HiFi polymerase	1 U/µl	0.5 U	
1.0	Indexed Adapter	10 µM	0.4 µM	
2.0	Purified template DNA			
14.5	Water			

Prepare mastermix in cold box and use repeater pipette to add to each tube in the cold box. Add Indexed Adapter to each tube.



🧪 5 μ L 5x KAPA HiFi Fidelity Buffer

🧪 1 μ L dNTP Mix

🧪 1 μ L Uni Adapter (ADPT_P1)

🧪 0.5 μ L KAPA HiFi polymerase

🧪 1 μ L Indexed Adapter

🧪 2 μ L Purified template DNA

🧪 14.5 μ L Water

39 **Cycle** (PCR machine #5 SZ $\rightarrow$ ILM2):

95°C	2 min
98°C	20 s
63°C	15 s
72°C	30 s
25 - 35 cycles	
72°C	3 min
4°C	On hold

Gel Purification and quantification

40 Before gel purification, run 2 μ L products on 1% agarose gel to check the bands.

41 **Gel purification.** (Qiagen QIAquick gel extraction kit)

Run 2nd round PCR products on 1.2% agarose gel. E = 4 V/cm, T = 60 min.

42 Excise DNA fragment.

43 Weight the gel; add 3 volume of Buffer QG to 1 volume of gel.

44 Incubate at 50 °C for **10 minutes** to completing dissolve. Vortex every **2-3 minutes** to help dissolve.



00:10:00 Incubation at 50 °C

00:02:30 Vortex

45 Check the color of gel solution (should be yellow, otherwise add 10 µl 3M sodium acetate).

46 Place **MinElute** column, apply the sample to the column and centrifuge for **1 minute**.

00:01:00 Centrifugation

47 Add 500 µl buffer QG and centrifuge for **1 minute**.

500 µL Buffer QG

00:01:00 Centrifugation

48 Add 0.75 ml buffer PE, **incubate for 5 minutes** at room temperature, centrifuge for **1 minute**.

00:05:00 Incubation at room temperature

00:01:00 Centrifugation

49 Discard the fluid, centrifuge for additional **3 minutes**.

00:03:00 Centrifugation

50 Put the column in a new 1.7 ml tube, add **10 µl** buffer EB. Stand for **4 minutes**, centrifuge for **2 minutes**.

00:04:00 Stand

51 Quantification using Invitrogen Qubit dsDNA BR Assay kit. See Qubit dsDNA BR assay protocol. **Don't use Nanodrop to quantify!**

52 After quantification, pool libraries in equal amount. Use AMPure XP beads to purify pooled libraries (2:3, two washes), elute in 20 to 30 µL Elution Buffer.

53 Quantify the pooled library using Qubit dsDNA BR assay kit. Check the quality of the library by Agilent Bioanalyzer or Bio-rad Experion. Repeat purification if primer dimer is present (~200bp).