



Apr 30, 2020 Version 2

🌐 Qant-iT™ PicoGreen® dsDNA Quantification V.2

📁 In 1 collection

DOI

dx.doi.org/10.17504/protocols.io.bftfjnjn

Roey Angel¹, Eva Petrova¹

¹Soil and Water Research Infrastructure

Anaerobic and Molecular Microbiology Lab, Biology Centre CAS
Tech. support email: eva.petrova@bc.cas.cz



Roey Angel

Soil and Water Research Infrastructure

SOWA

OPEN  ACCESS



DOI: dx.doi.org/10.17504/protocols.io.bftfjnjn

External link: <https://www.thermofisher.com/order/catalog/product/P11496>

Protocol Citation: Roey Angel, Eva Petrova 2020. Qant-iT™ PicoGreen® dsDNA Quantification. **protocols.io**
<https://dx.doi.org/10.17504/protocols.io.bftfjnjn>

Manuscript citation:

Angel, R., Claus, P., and Conrad, R. (2012). Methanogenic archaea are globally ubiquitous in aerated soils and become active under wet anoxic conditions. ISME J 6, 847–862. doi:10.1038/ismej.2011.141.

License: This is an open access protocol distributed under the terms of the **Creative Commons Attribution License**, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited

Protocol status: Working

We use this protocol and it's working

Created: April 30, 2020

Last Modified: April 30, 2020

Protocol Integer ID: 36423



Keywords: DNA, quantification, nucleic acids, fluorometric assay, high-throughput,

Abstract

The following protocol is intended for the quantification of double-stranded DNA using Quant-iT™PicoGreen® dsDNA Assay Kit (ThermoFisher). This protocol is a simplified and condensed version of the full protocol from the manufacturer. The procedure described here is for 96 reactions. If samples are run in duplicates, then this should allow quantifying 40 samples.

Attachments



[mp07581.pdf](#)

240KB

Materials

MATERIALS

Quant-iT™ PicoGreen™ dsDNA Assay Kit **Invitrogen - Thermo Fisher Catalog #P11496**

STEP MATERIALS

Quant-iT™ PicoGreen™ dsDNA Assay Kit **Invitrogen - Thermo Fisher Catalog #P11496**

Protocol materials

Quant-iT™ PicoGreen™ dsDNA Assay Kit **Invitrogen - Thermo Fisher Catalog #P11496**

Quant-iT™ PicoGreen™ dsDNA Assay Kit **Invitrogen - Thermo Fisher Catalog #P11496**

Quant-iT™ PicoGreen™ dsDNA Assay Kit **Invitrogen - Thermo Fisher Catalog #P11496**

Safety warnings

! Quant-iT™ PicoGreen® reagent is classified as Not Hazardous. Nevertheless, the user should always consult the MSDS accompanying any of the reagents and apparatus described in this protocol.



Before start

1. This protocol is optimised for measuring an entire 96-well plate. It assumes that 16 wells will be used for measuring the standards and the blank samples (in duplicates) and 80 wells will be used for measuring unknown DNA samples (typically in duplicates).
2. The protocol can be easily adjusted for a lower number of samples by reducing the volume of the working solutions of the reagents. Note though that enough TE should be retained for diluting the standard stock solution (490 or 680 μl), for potentially diluting the unknown samples, if their concentration is too high, and for accounting for pipetting errors. To fill the plate, 19.2 ml of TE is needed. So if only 40 wells are to be used for measuring unknown samples prepare about $50/96 \times 22 \approx 11.5$ ml of TE buffer.
3. The dynamic range of the assay is between 50 pg ml^{-1} to 1000 ng ml^{-1} . This translates into DNA sample concentrations of 0.05-5 $\text{ng } \mu\text{l}^{-1}$ and 1-200 $\text{ng } \mu\text{l}^{-1}$ in the low-range and high-range assays, respectively. Samples with higher DNA concentration need to be diluted (e.g. in DNase-free water or TE buffer).
4. Note that some compounds that can be present as DNA contaminations (e.g. salts, ethanol, detergents, proteins) are claimed by the manufacturer to not interfere with the measurement. Please refer to the full protocol for a list of these compounds and their effect on the measurement. Also, equimolar presence of ssDNA and RNA in the sample should have only minimal effect on the quantitation results.

Prepare reaction

53m

- 1 Take out all reagents from the fridge and bring them to room temperature. Take out the DNA samples from the freezer. DNA samples should be slowly thawed on ice.

20m



Note

Quant-iT™ PicoGreen® dsDNA reagent is dissolved in dimethylsulfoxide (DMSO), which freezes below 19 °C. The reagent must be completely thawed before using it by bringing it to room temperature. After the reagent thawed, it is advisable to briefly vortex the tube to make sure it is adequately mixed and to spin it down in a centrifuge or a mini centrifuge.

Note

Quant-iT™ PicoGreen® dsDNA reagent is light sensitive and should be protected from light at all times.





Quant-iT™ PicoGreen™ dsDNA Assay Kit **Invitrogen - Thermo**
Fisher Catalog #P11496

- 2 Prepare 22 ml 1X TE buffer by pipetting 1.1 ml of 20X TE buffer into 20.9 ml of nuclease-free water into a sterile and nuclease-free 50 ml tube. Mix by inverting the tube several times.

2m




 1.1 mL 20X TE buffer


 20.0 mL nuclease-free water

- 3 **For high-range quantification:**

2m

Dilute the DNA-standard stock solution (λ DNA 100 ng μL^{-1}) to a final concentration of 2 ng μL^{-1} by mixing 10 μL λ DNA-standard stock solution with 490 μL 1X TE buffer.

 10 μL λ DNA-standard stock solution

 490 μL 1X TE buffer

For low-range quantification:

Prepare a 40-fold dilution of the 2 ng μL^{-1} DNA-standard work solution by mixing 5 μL of the 2 ng μL^{-1} DNA-standard work solution with 195 μL 1X TE buffer to yield a 0.05 ng μL^{-1} DNA-standard work solution.



🧪 5 μL diluted DNA-standard solution

🧪 195 μL 1X TE buffer

- 4 If needed, prepare a dilution of each sample in 1X TE buffer so that the reading will be within the dynamic range.

Note

It is advisable to run samples in duplicates for a more accurate quantification

- 5 Prepare PicoGreen[®] work solution: 9950 μL 1X TE buffer + 50 μL PicoGreen[®] into a sterile and nucleic-acids free 50 ml tube. Mix and protect from light.

🧪 9950 μL 1X TE buffer

🧪 50 μL PicoGreen[®]

2m

- 6 Prepare the following standard mixture in the first two columns of the black, sterile, 96-well plate:

10m

Assay version	Diluted DNA std. (μL)	1X TE buffer (μL)	Final DNA amount (ng)
High-range (1-200 ng μL^{-1})	100	0	200
Use 2 ng μL^{-1} standard	50	50	100
	10	90	20
	1	99	1
	0	100	0
Low-range (50 pg μL^{-1} - 5 ng μL^{-1})	100	0	5
Use 0.05 ng μL^{-1} standard	50	50	2.5
	10	90	0.5
	1	99	0.05
	0	100	0

Equipment

96-well microtiter plate

NAME

Nunc

BRAND

265301

SKU

<https://www.thermofisher.com/order/catalog/product/152028#/152028>^{LINK}

black, flat bottom

SPECIFICATIONS

7 Pipette 99 µl of 1X TE buffer in the remaining wells.

5m

🧪 99 µL 1X TE buffer

Note

Tip: use a mechanical or electronic dispenser during this step and step no. 9 to speed up the work.

Equipment

Multipette E3

NAME

Eppendorf

BRAND

4987000010

SKU

<http://multipette-system.eppendorf.com/>

LINK

electronic dispenser

SPECIFICATIONS

8 Pipette 1 µl of the unknown DNA samples in the remaining wells.



 1 μL of DNA sample

10m

Note

Use either a diluted sample in case the concentration is expected to be higher than the dynamic range limit or larger volume in case the concentration is expected to be below the detection limit.


- 9 Pipette 100 μL of the PicoGreen[®] work solution in each well, including the standard and unknown sample wells.

2m

 100 μL PicoGreen work solution

- 10 Protect the 96-well plate from light and incubate for 2-5 min at room temperature.

5m

 00:02:00



Measure samples

5m

- 11 Place the plate in a plate reader and measure the fluorescence according to the following parameters:

5m



Excitation	~480 nm
Emission	~520 nm
Integration time	40 s
Lag time	0 s
Gain	Optimal
Number of flashes	10
Calculated well	highest standard
Shaking	5 s

Note

It is also possible to set the gain to a fixed value (e.g. 100). If the fluorescence values of the standard drop over time this could indicate damage to the reagents or the DNA standard.

Equipment

Synergy 2

NAME

absorbance microplate reader

TYPE

BioTek

BRAND

Synergy2


SKU

<https://www.biotek.com/products/detection/>

LINK

- 12 Plot the measured fluorescent values of the standard samples against their known concentrations and fit a linear curve using linear regression. Make sure that the coefficient of determination (R^2) is close to 1 (typically > 0.99). Calculate the DNA concentrations in the unknown samples using the slope and intercept parameters of the linear equation. Output values you obtained are in $\text{ng } \mu\text{l}^{-1}$, assuming $1 \mu\text{l}$ of each sample was used.

10m

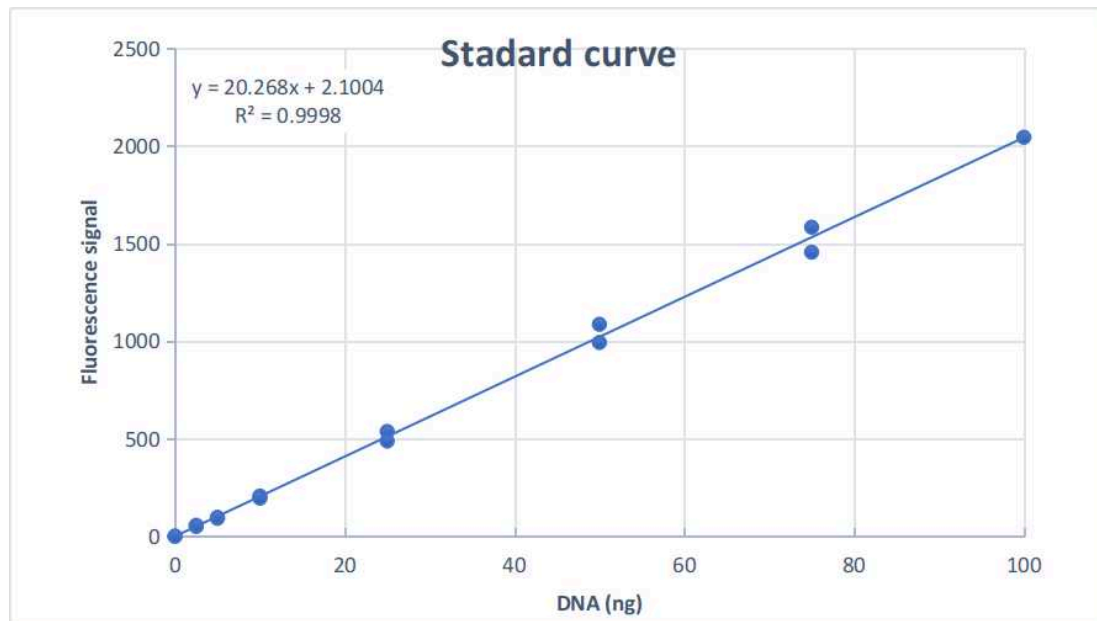



Note

Do not forget to account for any dilutions when calculating the concentration of the DNA in the unknown samples.



PicoGreen_example.xlsx