

Sep 10, 2020

Version 4

Qualitative & Quantitative Assessment of Human Islets for Distribution Using Dithizone (DTZ) V.4

 In 1 collection



DOI

dx.doi.org/10.17504/protocols.io.bk5vky66

Integrated Islet Distribution Program¹

¹Integrated Islet Distribution Program, City of Hope, Duarte, CA

Integrated Islet Distributi...

Integrated Islet Distributi...



Integrated Islet Distribution Program

Integrated Islet Distribution Program, City of Hope

Create & collaborate more with a free account

Edit and publish protocols, collaborate in communities, share insights through comments, and track progress with run records.

Create free account

OPEN  ACCESS



DOI: <https://dx.doi.org/10.17504/protocols.io.bk5vky66>

Protocol Citation: Integrated Islet Distribution Program 2020. Qualitative & Quantitative Assessment of Human Islets for Distribution Using Dithizone (DTZ). protocols.io <https://dx.doi.org/10.17504/protocols.io.bk5vky66> Version created by **Integrated Islet Distribution Program**



Manuscript citation:

License: This is an open access protocol distributed under the terms of the **Creative Commons Attribution License**, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited

Protocol status: Working

We use this protocol and it's working

Created: September 09, 2020

Last Modified: September 10, 2020

Protocol Integer ID: 41877

Keywords: Human Islets, Dithizone, Purity, Islet Equivalent, Actual Islet, Islet Quality Grade, Islet Index, Islets of Langerhans, human islets, islet equivalent, nih clinical islet transplantation consortium, quantitative assessment of human islet, sponsored clinical islet transplantation consortium phase, quantitative assessment of islet, zinc in the insulin granule, isolated islet preparation, islet cell, purified human pancreatic islet, integrated islet distribution program, research in the integrated islet distribution program, islet preparation, human islet, percent islet purity, islet equivalent, using dithizone, final islet product, pancreatic islet, islet quantity, quality of the final islet product, islet isolation center, participating islet isolation center, insulin granule, trapped islet, number of islet equivalent, islet, islet volume, dithizone, diphenyl thiocarbazon, assay method, dtz staining, dtz, diabetes, present in the beta cell, process assay, zinc, complex cellular product, beta cell, diameter of the isl

Abstract

This Standard Operating Procedure is adapted from the work of the 'National Institutes of Health-Sponsored Clinical Islet Transplantation Consortium Phase 3 Trial: Manufacture of a Complex Cellular Product at Eight Processing Facilities'' following the SOP cited in the document 'Purified Human Pancreatic Islet: Qualitative and Quantitative Assessment of Islets Using Dithizone (DTZ) – Standard Operating Procedure of the NIH Clinical Islet Transplantation Consortium'

This SOP defines the assay method for quantitative and qualitative determination in the identification of human isolated islet preparations, which include endocrine and exocrine tissue, for use in the National Institute of Diabetes and Digestive and Kidney Diseases (NIDDK) sponsored research in the Integrated Islet Distribution Program (IIDP). This protocol is written to assist the participating islet isolation centers and investigators who are part of this program.

Note

Notice: This SOP corrects an error which has been discovered on the conversion factor of islets to IEQ for the 101-150 range in Step 4.3 and on Attachment 1. The conversion factor should be 0.648 not 0.667. We apologize for the error, but the discrepancy in the conversion factor was difficult to trace historically, hence the importance for Rigor and Reproducibility provided by protocols.io. Documentation of this revision is found in Kin T. (2010) Islet Isolation for Clinical Transplantation. *The Islets of Langerhans. Advances in Experimental Medicine and Biology*. Volume 654. Dordrecht: Springer; p 683-710 referenced below.

Note

Integrated Islet Distribution Program (IIDP) (RRID:SCR_014387)

Dithizone (diphenyl thiocarbazon; DTZ) is an organic chemical that chelates the zinc in the insulin granules present in the beta cells of the pancreatic islets. The islet cells are stained red while the acinar cells remain unstained.

DTZ staining is used as a lot release and as an in-process assay:

(i) Lot release testing: DTZ staining is used to identify islets and to determine the quantity and quality of the final islet product. Islet quantity is expressed as the number of islet equivalents (IEQ), which is calculated based on the number and diameter of the islets present in the preparation, mathematically corrected for islet volume.

(ii) In-process testing: DTZ staining is used to identify islets and to assess the effectiveness of the digestion, isolation and purification processes. The quality of the preparations is expressed as percent islet purity, and percent trapped islets. Islet quantity (IEQ) is also assessed.

Guidelines

- **Integrated Islet Distribution Program (IIDP) (RRID:SCR_014387)**: The IIDP is a contracted program commissioned and funded by the NIDDK to provide quality human islets to the diabetes research community to advance scientific discoveries and translational medicine. The IIDP consists of the NIDDK, the Project Officer (PO), the External Evaluation Committee (EEC) and the CC at City of Hope (COH). The IIDP CC integrates an interactive group of academic laboratories including the subcontracted IIDP centers.
- **IIDP Coordinating Center (CC)**: Joyce Niland, Ph.D. is the Principal Investigator for the IIDP CC and leads staff from the Department of Research Information Sciences at COH to coordinate the activities of the IIDP and assist the participating centers and investigators in the distribution of human islets.
- **Percent Purity**: the percentage of islets compared to all tissue present in the islet preparation (islets, acinar and ductal cells) which is determined by visual inspection of a representative sample of the islet preparation. Islets are distinguished from non- islet tissue by using Dithizone (DTZ) to stain red the zinc granules in the beta cells.
- **Actual Islets (AI) or Islet Particle Number (IPN)**: The actual number of islets or islet particles counted. For this SOP, the nomenclature of Actual Islets (AI) will be used.
- **Islet Equivalent (IEQ)** : An IEQ is defined as an islet with a diameter of 150 microns. The number of IEQ in each size class is calculated by multiplying the number of islets by a conversion factor for each size.
- **Islet Quality Grade**: A qualitative designation given to the islet preparation after microscopic evaluation based on the parameters of shape, border, integrity, number of single cells, and overall islet diameter.
- **Equations for Total Equivalent (Total IEQ) and Total Actual Islet(AI)**:
 1. **Total IEQ** = Dilution Factor x
[(AI of diameter 50 – 100 μ m x 0.167) +
(AI of diameter 101 – 150 μ m x 0.648) +
(AI of diameter 151 – 200 μ m x 1.685) +
(AI of diameter 201 – 250 μ m x 3.500) +
(AI of diameter 251 – 300 μ m x 6.315) +
(AI of diameter 301 – 350 μ m x 10.352) +
(AI of diameter > 350 μ m x 15.833)]
 2. **Total AI** = Dilution Factor x \sum AI of each diameter
- **Islet Index (II)**: A quantitative designation given to the islet preparation after microscopic evaluation determined by dividing the IEQ by the AI. This designation determines the overall size distribution of the islets being shipped. If the majority of AI is around 150 μ m (1-IEQ) then the II will equal 1.0. If the majority of AI is larger than 150 μ m, then the II will be > 1.0. If the majority of the AI is smaller than 150 μ m, then the II will be <1.0.

References:



Citation

Ricordi, C. Gray, D. W. Hering, B. J. Kaufman, D. B. Warnock, G. L. Kneteman, N. M. Lake, S. P. London, N. J. Socci, C. Alejandro, R. et al.,
(1990). Islet isolation assessment in man and large animals. Acta Diabetol Lat, Vol 27, Issue 3, Pg 185-95.

<https://doi.org/10.1007/BF02581331>

LINK

Citation

Ricordi, C (1992). Pancreatic Islet Cell Transplantation. Austin: R.G. Landes Company.

Citation

Kin T. (2010). Islet Isolation for Clinical Transplantation.
The Islets of Langerhans. Advances in Experimental Medicine and Biology. Volume 654. Dordrecht: Springer; p 683-710.



Citation

NIH CIT Consortium Chemistry Manufacturing Controls Monitoring Committee, NIH CIT Consortium (2015)
. Purified Human Pancreatic Islet: Qualitative and Quantitative Assessment of Islets Using Dithizone (DTZ): Standard Operating Procedure of the NIH Clinical Islet Transplantation Consortium.
CellR4-- repair, replacement, regeneration, & reprogramming.

<https://doi.org/pii:e1369>

LINK

Citation




Ricordi C, Goldstein JS, Balamurugan AN, Szot GL, Kin T, Liu C, Czarniecki CW, Barbaro B, Bridges ND, Cano J, Clarke WR, Eggerman TL, Hunsicker LG, Kaufman DB, Khan A, Lafontant DE, Linetsky E, Luo X, Markmann JF, Naji A, Korsgren O, Oberholzer J, Turgeon NA, Brandhorst D, Chen X, Friberg AS, Lei J, Wang LJ, Wilhelm JJ, Willits J, Zhang X, Hering BJ, Posselt AM, Stock PG, Shapiro AM, Chen X
(2016)
. National Institutes of Health-Sponsored Clinical Islet Transplantation Consortium Phase 3 Trial: Manufacture of a Complex Cellular Product at Eight Processing Facilities.
Diabetes, 2016 Nov, 65(11): 3418-28. PMCID: 5079635.


<http://www.ncbi.nlm.nih.gov/pubmed/27465220>

LINK

Materials

MATERIALS

-  Dithizone (Diphenylthiocarbazone) **Merck MilliporeSigma (Sigma-Aldrich) Catalog #D5130**
-  Gibco DPBS without Calcium and Magnesium **Fisher Scientific Catalog #14190136 or equivalent**
-  Dimethyl sulfoxide **Merck MilliporeSigma (Sigma-Aldrich) Catalog #D8779 or equivalent**

Equipment	
Gilson™ PIPETMAN Classic™ Pipets- F123601 or equivalent	NAME
Adjustable pipettor -P200	TYPE
Gilson	BRAND
F123601G	SKU
https://www.fishersci.com/shop/products/gilson-pipetman-classic-pipets-model-p200-vol-50-200-l/f123601g	LINK
50 to 200µL, ±0.5, ±1µL	SPECIFICATIONS
	

Equipment

Fisherbrand™ Large-Orifice Pipet Tips, 1 to 200µL or equivalent

NAME

Genomic/Wide Orifice Pipet Tips

TYPE

Fisherbrand

BRAND

02-707-134

SKU

<https://www.fishersci.com/shop/products/fisherbrand-large-orifice-pipet-tips-6/02707134?keyword=true>

LIN
K

1 to 200µL

SPECIFICATIONS



Equipment

Fisherbrand™ Petri Dishes with Clear Lid or equivalent

NAME

Petri Dishes

TYPE

Fisherbrand

BRAND


FB0875713A

SKU

<https://www.fishersci.com/shop/products/fisherbrand-petri-dishes-clear-lid-12/fb0875713a> ^{LINK}

Round, Raised Ridge, 60mm, 15mm

SPECIFICATIONS



Equipment

Thermo Scientific™ Nalgene™ Rapid-Flow™ Sterile Disposable Bottle Top Filters with PES Membrane or equivalent

NAM
E

0.45 um Bottle Top filter

TYPE

Thermo Scientific

BRAND

09-740-62C

SKU

<https://www.fishersci.com/shop/products/nalgene-rapid-flow-sterile-disposable-bottle-top-filters-pes-membrane/0974062c> ^{LINK}


0.45µm nylon Filter


SPECIFICATIONS



Equipment	
Invitrogen™ EVOS™ XL Core Imaging System or equivalent	NAME
Inverted Microscope	TYPE
Light Microscope	BRAND
AMEX1000	SKU
https://www.fishersci.com/shop/products/evos-xl-core-imaging-system/12562751#?keyword=Inverted+Microscopes	LINK

Equipment	
Lab inverted light microscope	NAME
Eyepiece with Calibrated reticle, 1mm	BRAND
Microscope specific, lab SOP	SKU

Equipment	
Bal Supply Cell Counter or equivalent	NAME
Cell Counter (Manual or Electronic)	TYPE
Bal Supply	BRAND
02-670-14	SKU
https://www.fishersci.com/shop/products/bal-supply-cell-counters-4/0267014	LINK
	

Equipment	
Drummond™ Fixed-Volume Microdispensers or equivalent	NAME
Drummond 3000385	TYPE
Drummond™	BRAND
21176F	SKU
https://www.fishersci.com/shop/products/drummond-fixed-volume-microdispensers-16/21176f?searchHijack=true&searchTerm=21176F&searchType=RAPID&matchedCatNo=21176F	LINK
Volumetric Range 100/200UL with borosilicate glass bores	SPECIFICATIONS
	

Equipment

new equipment

NAME

Computer or calculator or equivalent

BRAND

NA

SKU

Computer software (e.g. Excel) with the mean and standard deviation functions

SPECIFICATIONS

Troubleshooting

Safety warnings



Dimethyl sulfoxide (DMSO)



DMSO_MSDSAAction.pdf

- Hazard statement(s): Combustible liquid.
- Precautionary statement(s): Keep away from heat/sparks/open flames/hot surfaces. No smoking. Wear protective gloves/ protective clothing/ eye protection/ face protection.
- DMSO itself is not toxic but it can be a carrier of chemicals, viruses, etc. into the skin

Dithizone (DTZ)






Dithizone_MSDSAAction.pdf

- Hazard Statement(s): Causes skin irritation. Causes serious eye irritation.
- Precautionary statement(s): Wash skin thoroughly after handling. Wear protective gloves/ eye protection/ face protection.



Preparation of Working Dithizone

- 1 Assemble all items described in the Materials section.
- 2 Prepare DTZ stain as described below. Observe all safety precautions when working with DMSO.
 - 2.1 Dissolve  50 mg dithizone in  10 mL DMSO.
 - 2.2 Add DPBS to bring the total volume to  50 mL .
 - 2.3 Filter the combined solution using a 0.45 µm nylon filter.
 - 2.4 Place solution in a 50 mL conical tube and label "Dithizone Stain or DTZ" with:
 - Preparation Date and Time
 - **Expiration Date and Time (24 hours after preparation)**
 - Initials of person preparing solution

Preparation of Islets for Counting

- 3 Samples for islet quantitation and purity should be taken for islet broadcast either after the isolation or post culture. Sampling must be repeated prior to packaging for shipment in order to ensure that samples after culture are representative of what is being distributed to the investigators.
 - 3.1 Mix the final islets suspension very gently but thoroughly by inverting the islet prep in a conical 2-3 times before quickly taking a sample. (Do not swirl.) As islets settle rapidly, care must be taken to ensure a representative sample is taken from the middle of the suspension.




- 3.2 Take replicate 100–200 μL sample volumes from 100 mL final prep using a widebore tip pipettor. Two duplicate counts should be performed by two separate technicians or 2 separate counts by one technician.
- 3.3 Add 3 drops (30 μL) of the DTZ solution to the islets sample and allow staining for 1 – 2 minutes at room temperature. Cover the bottom of the counting dish with DPBS to approximately $\frac{1}{2}$ the height of the dish. Count the islets under the microscope following the steps below.



Islet Quantification

4 Identify AI, IEQ, and % purity.

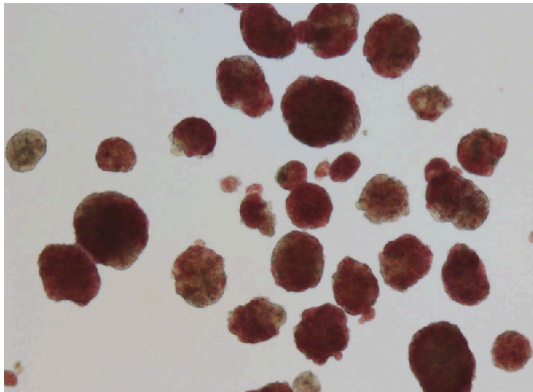

Dithizone Stained Islets

Note

Dithizone (diphenyl thiocarbazon; DTZ) is an organic chemical that chelates the zinc in the insulin granules present in the beta cells of the pancreatic islets. *The islet cells are stained red while the acinar cells remain unstained.*

- Islets are counted by size of the Actual Islets (AI), tabulated, and mathematically calculated to determine the Total Islet Equivalents (IEQ).
- Examine the islets sample (***stained islets will appear red***) using the 10x eyepiece and the 4x objective to give a total magnification of 40x.
- Using the grid lines on the counting dish as a guide, methodically scroll through the dish from side to side, and top to bottom, examining each islet.

- Count islets within the perimeter of the grid's squares, including only islets touching the top and right lines (not the bottom and left lines), to avoid counting the same islet twice.

4.1 There are different types of reticles that can be used but all should be certified in the eyepiece to the correct specification by the microscope company representative. Once calibrated, the eyepiece of the microscope is used to determine the size of each islet.

Using the table below as a guide, regardless of which type of reticle is used, count (tally) the number of Actual Islets (AI) in each diameter group using the manual or electronic cell counter. Do not count islets smaller than 50 μm because their contribution is not significant.

Number of Spaces Spanned	Diameter of Islet (μm)
< 2	< 50
2 – 4	50 – 100
4 – 6	101 – 150
6 – 8	151 – 200
8 – 10	201 – 250
10 – 12	251 – 300
12 – 14	301 – 350
> 14	> 350

4.2 Calculate the dilution factor as follows:

Example for a 100 μL sample from a 100 mL total volume =1000 dilution factor

Expected result

Dilution Factor = [(mL total volume / μL sample volume) X 1000]

4.3 Record and calculate the results using Excel Spreadsheet in Attachment 1.





Expected result

Islet Diameter Range (μm)	Islet Particle Number (IPN)	IEQ Conversion Factor	IEQ per Range
50 – 100	11	X 0.167	1.84
101 – 150	42	X 0.648	27.22
151 – 200	26	X 1.685	43.81
201 – 250	13	X 3.500	45.50
251 – 300	5	X 6.315	31.58
301 – 350	0	X 10.352	0.00
>350	1	X 15.833	15.83
Σ AI	95	Σ IEQ	165.77
Dilution Factor [(mL total volume / μL sample volume) X 1000]			1000
Total AI = Σ AI X Dilution Factor			98,000
Total IEQ = Σ IEQ X Dilution Factor			165,771

Example for a 100 μL sample from a 100 mL total volume

- Calculate the Total Actual Islets (Σ AI), and the Total Islet Equivalentents (Σ IEQ) by inputting the data from the tally, in step 4.1, into the Excel spreadsheet in Attachment 1 for Most Pure Shipment and Least Pure Shipment if applicable.
- Calculate the total number of IEQ present by entering the total Actual Islets (AI) in each range which will be converted using the conversion factor, to IEQ per each range. This conversion normalizes the AI to 150 μm sized islet.
- Both the AI and IEQ will be totaled and multiplied by the dilution Factor for a Final AI count and Final IEQ Count of the preparation.
- The Islet Index (II), a calculation made by dividing the IEQ by the AI, is calculated automatically in Attachment 1. This designation determines the overall size distribution of the islets being shipped.
- Repeat process, as needed, for a Least Pure Shipment.



Attachment 1-Islet Tabulation Coun...

Islet Quality Grade by Islet Ranking

- 5 Determine the Islet Quality Grade based on the chart below and Islet Ranking Guide (Attachment 2). Record and calculate the results on Attachment 1 for Most Pure Shipment and Least Pure Shipment, if applicable, and on broadcast website.



Attachment 2-Islet Ranking Guide.p...

Parameter	0 Points	1 Point	2 Points
Shape (3D)	flat/planar	in between	spherical
Border (2D)	irregular	in between	well-rounded
Integrity	fragmented	in between	Solid/compact
Single Cells	many	a few	almost none
Diameter	all<100µm	a few>200 µm	>10%>200 µm

Islet Purity

- 6 Calculate the percent purity of the islets to the nearest 5% by estimating the portion of dithizone (red stained islets) to all tissue (islets, acinar, ductal cells). Record the purity of each sample on Attachment 1. The average will be calculated automatically.



Photographic Documentation

- 7 Take digital images and upload (when applicable) for IIDP Islet Broadcast of the count sample.
- 7.1 Gently swirl the count sample in order to center the islets in the dish. This will give a representative photographic image of the purity and size distribution of the islet preparation. If possible, take a well focused digital photo, using the center's SOP for it's specific microscope and camera set-up, so the final image size is a 10x-40x magnification. Label and save image with RRID#, date, time when photo was taken (prior to broadcast), and magnification.



- 7.2 With the use of the digital imaging techniques on the IIDP website, upload images and match the background grid lines per the online instructions in the broadcast section (when applicable).

Subsequent Counting, Grading, Purity, and Viability

- 8 Repeat all counting, grading, purity, and viability estimates and digital image uploads for islets prior to packaging for distribution if more than 6 hours post original broadcast evaluations. Update broadcast records under the "Confirm Islet Information" section of the broadcast and repeat these procedures for rebroadcasts and shipments with every subsequent 24 hour rebroadcast/shipment.

Citations

Ricordi, C. Gray, D. W. Hering, B. J. Kaufman, D. B. Warnock, G. L. Kneteman, N. M. Lake, S. P. London, N. J. Socci, C. Alejandro, R. et al.,. Islet isolation assessment in man and large animals

<https://doi.org/10.1007/BF02581331>

Ricordi, C. Pancreatic Islet Cell Transplantation

Kin T.. Islet Isolation for Clinical Transplantation

NIH CIT Consortium Chemistry Manufacturing Controls Monitoring Committee, NIH CIT Consortium. Purified Human Pancreatic Islet: Qualitative and Quantitative Assessment of Islets Using Dithizone (DTZ): Standard Operating Procedure of the NIH Clinical Islet Transplantation Consortium

<https://doi.org/pii:e1369>

Ricordi C, Goldstein JS, Balamurugan AN, Szot GL, Kin T, Liu C, Czarniecki CW, Barbaro B, Bridges ND, Cano J, Clarke WR, Eggerman TL, Hunsicker LG, Kaufman DB, Khan A, Lafontant DE, Linetsky E, Luo X, Markmann JF, Naji A, Korsgren O, Oberholzer J, Turgeon NA, Brandhorst D, Chen X, Friberg AS, Lei J, Wang LJ, Wilhelm JJ, Willits J, Zhang X, Hering BJ, Posselt AM, Stock PG, Shapiro AM, Chen X. National Institutes of Health-Sponsored Clinical Islet Transplantation Consortium Phase 3 Trial: Manufacture of a Complex Cellular Product at Eight Processing Facilities

<http://www.ncbi.nlm.nih.gov/pubmed/27465220>