




May 23, 2025

Version 1

Usutu virus (Orthoflavivirus usutuense) amplicon sequencing for Illumina V.1

DOI

<https://dx.doi.org/10.17504/protocols.io.eq2lyjormlx9/v1>



Gábor óth¹, Marike Petersen¹, Alexandra Bialonski¹, Heike Baum¹, Marcy A. Sikora¹, Alex Tomazatos¹, Balázs orváth¹, Jonas Schmidt-Chanasit¹, Dániel adar¹

¹Bernhard Nocht Institute for Tropical Medicine



Dániel Cadar

BNITM

Create & collaborate more with a free account

Edit and publish protocols, collaborate in communities, share insights through comments, and track progress with run records.

Create free account

OPEN  ACCESS



DOI: <https://dx.doi.org/10.17504/protocols.io.eq2lyjormlx9/v1>

Protocol Citation: Gábor óth, Marike Petersen, Alexandra Bialonski, Heike Baum, Marcy A. Sikora, Alex Tomazatos, Balázs orváth, Jonas Schmidt-Chanasit, Dániel adar 2025. Usutu virus (Orthoflavivirus usutuense) amplicon sequencing for Illumina. protocols.io <https://dx.doi.org/10.17504/protocols.io.eq2lyjormlx9/v1>



License: This is an open access protocol distributed under the terms of the **Creative Commons Attribution License**, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited

Protocol status: In development

We are still developing and optimizing this protocol

Created: March 04, 2024

Last Modified: May 23, 2025

Protocol Integer ID: 96095

Keywords: WNV, West Nile virus, Targeted Sequencing, Illumina, iSeq100, Lineage-2, usutu virus, many human pathogenic virus, orthoflavivirus usutuense, ebola virus, widespread arbovirus, methods for usuv, important virus, zika virus, sequencing method, usuv, natural circulation of usuv, illumina amplicon, virus, sequencing, illumina iseq, humans via mosquito bite, iseq100, illumina platform, illumina platform on the market, illumina, mosquito bite, molecular epidemiology, shorter amplicon length

Abstract

Amplicon based targeted sequencing methods proved their importance in case of many human pathogenic viruses (e.g. Zika virus, Ebola virus, SARS-Cov 2). Application and development of this methods for other medically important viruses could be also beneficial as it ensure the possibility of molecular epidemiology. Usutu virus (USUV, *Orthoflavivirus usutuense*) is widespread arbovirus which is mainly transmitted to humans via mosquito bites. In the natural circulation of USUV multiple hosts are involved which raise the need for sufficient sequencing method.

There are already available, established targeted sequencing methods for USUV, but we wanted to develop an additional one which uses shorter fragment length and optimised for Illumina iSeq 100. Shorter amplicon length works better on low quality samples and iSeq100 is the cheapest (most accessible) Illumina platform on the market.

Materials

A	B	C
Reagents		
Component	Supplier	Catalog number
QIAamp Viral RNA Mini Kit	Qiagen	52904
RealStar® WNV RT-PCR Kit 2.0	altona Diagnostics GmbH	322013
SuperScript IV Reverse Transcriptase	Invitrogen	18090010
Random Hexamers (50 µM)	Invitrogen	N8080127
RNaseOUT™ Recombinant Ribonuclease Inhibitor	Invitrogen	10777019
Q5® High-Fidelity DNA Polymerase	New England Biolabs	M0491S
dNTP Mix (10 mM each)	Thermo Scientific™	R0192
Individual primers	IDT or Eurofins etc.	
NEBNext® Ultra™ II End Repair/dA-Tailing Module	New England Biolabs	E7546S
QIAseq FX DNA Library UDI Kit (24)	Qiagen	180477
Agencourt® AMPure® XP	Beckman Coulter	A63880
Qubit™ 1X dsDNA High Sensitivity (HS)	Invitrogen	Q33230
Absolute Ethanol (Molecular Biology Grade)	any	-
Nuclease free water	any	-
SeaKem® LE Agarose	Lonza	50004
iSeq 100 i1 Reagent v2 (300-cycle)	Illumina	20031371
Consumables		
Qubit™ Assay Tubes	Invitrogen	Q32856
PCR tubes 0,2 ml	any	-



	A	B	C
	1,5 ml tubes	any	-
	Pipette tips 0,1-1000 µl		
	Equipments		
	Magnetic stand or rack	any	-
	Pipettes 0,1-1000 µl	any	-
	Qubit™ 4 Fluorometer	Invitrogen	Q33238
	End-point PCR machines	any	-
	Gel electrophoresis system	any	-
	iSeq 100 System	Illumina	

Safety warnings

- ❗ Multiplex PCR based amplification of a targeted pathogen genome could be highly effective, so it could serve as potential contamination source! This and other amplicon based method should be separated from diagnostic units to avoid cross-contamination. The implementation of negative controls are necessary to check the reagents purity.

Nucleic Acid Extraction

- 1 RNA extraction with QIAamp Viral RNA kit based on manufacturers recommendation. Other RNA extraction kits can be used as well e.g. *Quick-RNA Viral Kit* (Zymo Research).

Note

QIAamp® Viral RNA Mini Handbook



HB-0354-008_HB_QA_Viral_RNA_...

qRT-PCR

- 2 In house method with Jonas original primers. 2xQuantiTect Master Mix

45m 55s

Component Volume

2xQuantiTect Master Mix	5 µL
QuantiTect RT Mix	0.2 µL
Water	2 µL
Usutu F8	1.2 µL
Usutu R8	1.2 µL
Usutu P8	0.6 µL
Sample	5 µL

Final volume 20 µL

Reaction conditions

Step	Temperature	Time	Cycles
Reverse transcription	50 °C	00:30:00	1
Denaturation	95 °C	00:15:00	1
	95 °C	00:00:15	45

Amplification	🌡️ 52 °C	🕒 00:00:20	45
	🌡️ 72 °C	🕒 00:00:20	45

Note

In house protocol with a single modification. Increased sample volume 5 ul

Reverse transcription

3 Reverse transcription is conducted with SuperScript IV Reverse Transcriptase.

3.1 Mix the following components in a 0.2 mL tube.

Component	Volume
50µM random hexamers	🧴 1 µL
10mM dNTPs mix (10mM each)	🧴 1 µL
Template RNA	🧴 11 µL
Total volume	🧴 13 µL

3.2 Gently mix by pipetting, and spin down afterwards if needed. Incubate the reaction as follows:

6m

Temperature	Time
🌡️ 65 °C	🕒 00:05:00
Place on ice for	🕒 00:01:00

**Note**

The master mix should be prepared in a clean cabinet while the sample should be added in another one.

3.3 Prepare the following master mix:**Component****Volume**

SSIV Buffer

 4 μL

100mM DTT

 1 μL

RNaseOUT RNase Inhibitor

 1 μL

SSIV Reverse Transcriptase

 1 μL

Total volume

 7 μL

Add 7 μL of master mix to the 13 μL annealed template RNA. The final volume is 20 μL . Gently mix by pipetting, and spin down afterwards if needed.

3.4 Incubate the reaction as follows:

1h 15m

Temperature Time

25 °C 00:05:00

50 °C 00:50:00

70 °C 00:20:00

Note

The master mix should be prepared in a clean cabinet while the sample should be added in another one.

Primer pool preparation

- 4 Primer pool preparation from preordered primers. The primers were designed with the usage of Primalscheme using the sequences from the list below:

4.1 The list of designed primers and pool ID (1 or 2) are available in the attached table.

This table contains the necessary amount and ratios of individual primers what should be used for primer pool generation.

4.2 Primers should be sorted based on there pool ID and resuspend lyophilised oligos in nuclease free water to 100 μM concentration. We tried to optimise the primer concentrations and the current ratios are written in the table above. Use the mentioned amount ( 5 μL to  12.5 μL) from unique primers to generate primer stocks (Pool 1-2).

4.3 Dilute the primer stocks (100 μM cc) 1:10 in nuclease free water to get the reaction ready primer solution (10 μM).

Note

Primer pools should be prepared in a clean mastermix cabinet!

For one reaction  2.5 μL reaction ready primer solution (10 μM) is needed. It can be prepared and aliquoted in  100 μL to avoid contamination and degradation.

Multiplex-PCR

5 Set up the multiplex PCR reaction in 0.2 mL PCR tube.

Reactions with Pool 1 and 2 primers:

Component	Pool 1	Pool 2
5X Q5 Reaction Buffer	 5 μL	 5 μL
10 mM dNTPs	 0.5 μL	 0.5 μL
Q5 Hot Start DNA Polymerase	 0.25 μL	 0.25 μL
Primer Pool 1 or 2 (10 μM)	 2.5 μL	 2.5 μL
Nuclease-free water	 14.25 μL	 14.25 μL

Total volume:

🧴 22.5 µL

🧴 22.5 µL

Note

The master mix should be prepared in a clean cabinet while the sample should be added in another one.

- 6 Add 🧴 2.5 µL cDNA directly to each tube and mix well by pipetting. The final volume is 🧴 25 µL .

Note

Inside the extraction and sample addition cabinet

- 7 Set-up the following program on the thermal cycler:

2m 5s

Step	Temperature	Time	Cycles
Initial Denaturation	🌡️ 98 °C	🕒 00:00:30	1
Denaturation	🌡️ 98 °C	🕒 00:00:05	20-38
Annealing + Extension	🌡️ 60 °C	🕒 00:01:30	20-38
Hold	🌡️ 4 °C	Till further processes	

Note

The cycle number are determined based on the qPCR result. In our case the Ct number + ~3 cycles formula gave the best result (e.g. The Ct value is 26,54 use 30 cycles). In general, use higher number of cycles than the obtained Ct value.

This is a safe stopping point. The amplicons can be stored at 4°C till further processes.

Quantification and normalisation

- 8 Quantify  1 μL directly from the two different PCR reaction (Pool 1, Pool 2) with the 1x dsDNA HS Assaykit.
- 8.1 Aliquot  199 μL 1x Working solution to Qubit assay tube (equal to the number of your samples). Prepare two extra tubes for the standards with  190 μL 1x Working solution.
- 8.2 Add  1 μL sample for each test tube and  10 μL from the Standards (Standard 1, Standard 2). The final volume is  200 μL .
- 8.3 Mix each sample vigorously by vortexing and pulse centrifuge to collect the liquid.
- 8.4 Incubate at room temperature for  00:02:00 before measuring. 2m
- 8.5 Calibrate Qubit fluorometer with the standards based on manufacturers recommendation.
- 8.6 Read your sample.
- 8.7 Normalization is not required if the concentrations of the two reactions (Pool 1, Pool 2) from the same sample differ by 20 % or less. If the difference exceeds this threshold, use the entire volume of the low concentration pool and add an equivalent concentration from the other pool.

Note

Alternative dsDNA quantification systems can be used as well (e.g. QuantiFluor[®] ONE dsDNA System).



Amplicon clean-up

9 Conduct clean-up with Ampure XP Beads.

Sample/Bead ratio = 1:1 ( 50 μ L)

Washing: two times with  200 μ L 80% EtOH.

Elution:  28 μ L nuclease-free water.

9.1 Merge the two pools prior to adding the magnetic beads.

9.2 Add  50 μ L AMPure XP beads to the sample and mix gently. The sample/magnetic bead ratio is 1:1.

9.3 Incubate for  00:05:00 at room temperature.

5m

9.4 Place the tube on a magnetic rack for  00:02:00 (until supernatant is completely clear).

2m

9.5 Remove supernatant without touching the bead pellet.

9.6 Add  200 μ L freshly prepared 80% ethanol to the tube. Float the beads through ethanol either by replacing to another magnetic rack or mix via pipetting.

9.7 Remove supernatant and discard.

9.8 Repeat washing step with 80% ethanol (step 9.6-9.7).

9.9 Carefully remove the supernatant and dry the beads for around  00:02:00 by leaving the lid open. (Dull pellet indicates dryness)

2m



- 9.10 Remove tube from the magnetic rack and resuspend the pellets in $28\ \mu\text{L}$ nuclease-free water and incubate at room temperature for 00:02:00 . 2m
- 9.11 Place the tube back to a magnetic rack for 00:02:00 until supernatant is completely clear and transfer eluate into clean tube. Make sure that no beads are transferred as well. 2m

Quantification and normalisation

- 10 Quantify $1\ \mu\text{L}$ directly from the two different PCR reaction (Pool 1, Pool 2) with the 1x dsDNA HS Assaykit.
- 10.1 Aliquot $199\ \mu\text{L}$ 1x Working solution to Qubit assay tube (equal to the number of your samples). Prepare two extra tubes for the standards with $190\ \mu\text{L}$ 1x Working solution.
- 10.2 Add $1\ \mu\text{L}$ sample for each test tube and $10\ \mu\text{L}$ from the Standards (Standard 1, Standard 2). The final volume is $200\ \mu\text{L}$.
- 10.3 Mix each sample vigorously by vortexing and pulse centrifuge to collect the liquid.
- 10.4 Incubate at room temperature for 00:02:00 before measuring.
- 10.5 Calibrate Qubit fluorometer with the standards based on manufacturers recommendation.
- 10.6 Read your sample.
- 10.7 Normalization is not required if the concentrations of the two reactions (Pool 1, Pool 2) from the same sample differ by 20 % or less. If the difference exceeds this threshold, use the entire volume of the low concentration pool and add an equivalent concentration from the other pool.

Note

Alternative dsDNA quantification systems can be used as well (e.g. QuantiFluor® ONE dsDNA System).

End Repair and dA Tailing

11 Amplicon end preparation with NEBNext Ultra II End Repair/dA-Tailing Module.

11.1 Add the following components to a sterile nuclease-free tube:

Component	Volume
NEBNext Ultra II End Prep Reaction Buffer	3.5 µL
NEBNext Ultra II End Prep Enzyme Mix	1.5 µL
100 ng Amplicons	x µL
Nuclease-free water	25-x µL
Total volume	30 µL

Note

If the concentration does not reach the 4 ng / µl use the whole amount (25 µL) from the cleaned up amplicons.

11.2 Place sample in a thermal cycler, with the heated lid set to 75 °C , and run the following program:

45m

Temperature Time

20 °C 00:30:00

70 °C 00:15:00



Adapter Ligation

12 Adapter ligation with QIAseq FX DNA Library Kit.

12.1	Component	Volume
	DNA Ligase Buffer, 5x	 20 µL
	DNA Ligase	 10 µL
	UDI Adapter	 5 µL
	Nuclease-free water	 35 µL
	Previous reaction	 30 µL
	Final volume	 100 µL

12.2 Place sample in a thermal cycler without heated lid, set and incubate:

15m

Temperature **Time**

 20 °C

 00:15:00

Note

We used QIAseq FX DNA Library Kit as ligation module. Applied concentrations and reaction conditions are optimised for this protocol. Alternative ligase modules could be use after optimisation (e.g. from NEB).

Library clean up

13 Conduct clean-up with Ampure XP Beads.

Sample/Bead ratio = 1 : 0.6 ( 60 µL)

Washing: two times with  200 µL 80% EtOH.

Elution:  26 µL nuclease-free water.



- 13.1 Add  60 μL AMPure XP beads to the sample and mix gently. The sample/magnetic bead ratio is 1:0.6.
- 13.2 Incubate for  00:05:00 at room temperature.
- 13.3 Place the tube on a magnetic rack for  00:02:00 (until the supernatant is completely clear).
- 13.4 Remove supernatant without touching the bead pellet.
- 13.5 Add  200 μL freshly prepared 80% ethanol to the tube. Float the beads through ethanol either by replacing to another magnetic rack or mix via pipetting.
- 13.6 Remove supernatant and discard.
- 13.7 Repeat washing step with 80% ethanol (step 12.5-12.6).
- 13.8 Carefully remove the supernatant and dry the beads for around  00:02:00 by leaving the lid open. (Dull pellet indicates dryness)
- 13.9 Remove tube from the magnetic rack and resuspend the pellets in  26 μL nuclease-free water and incubate at room temperature for  00:02:00 .
- 13.10 Place the tube back to a magnetic rack for  00:02:00 until the supernatant is completely clear and transfer eluate into clean tube. Make sure that no beads are transferred as well.

Library amplification

- 14 Conduct library amplification with the usage of HiFi PCR Master Mix.

14.1 Mix the following components in an 0.2 mL tube.

Component	Volume
HiFi PCR Master Mix, 2x	 25 µL
Primer Mix Illumina Library Amp	 1.5 µL
Adapter ligated amplicons	 23.5 µL
Final volume	 50 µL

14.2 Step	Temperature	Time	Cycles	5m 20s
Initial Denaturation	 98 °C	 00:02:00	1	
Denaturation	 98 °C	 00:00:20	4-8	
Annealing	 60 °C	 00:01:30	4-8	
Extension	 72 °C	 00:00:30	4-8	
Final extension	 72 °C	 00:01:00	1	
Hold	 4 °C	Till further processes		

Note

<0,5 ng 8 cycle RIZSA

Final Library clean up

15 Conduct clean-up with Ampure XP Beads.

Sample/Bead ratio = 1 : 0.7 ( 35 µL)

Washing: two times with  200 µL 80% EtOH.

Elution:  50 µL Elution Buffer.




- 15.1 Add  35 μL AMPure XP beads to the sample and mix it gently. The sample/magnetic bead ratio is 1:0.7.
- 15.2 Incubate for  00:05:00 at room temperature.
- 15.3 Place the tube on magnetic rack for  00:02:00 (until the supernatant is completely clear).
- 15.4 Remove supernatant without touching the bead pellet.
- 15.5 Add  200 μL freshly prepared 80% ethanol to the tube. Float the beads through ethanol either by replacing to another magnetic rack or mix via pipetting.
- 15.6 Remove supernatant and discard.
- 15.7 Repeat washing step with 80% ethanol (step 14.5-14.6).
- 15.8 Carefully remove the supernatant and dry the beads for around  00:02:00 by leaving the lid open. (Dull pellet indicates dryness)
- 15.9 Remove tube from the magnetic rack and resuspend the pellets in  50 μL elution buffer and incubate at room temperature for  00:02:00 .
- 15.10 Place the tube back to the magnetic rack for  00:02:00 until the supernatant is completely clear and transfer the eluate into clean tube. Make sure that no beads are transferred as well.

Library Size check

- 16 Run  10 μL from the cleaned up final library on 1,5% agarose gel. Low concentration of WNV genome in the sample could affect the multiplex PCR effectivity. Missing

template genome results high amount of primer dimers. The expected final library size is 400bp to 420 bp. The dimers are appearing around 200 bp.

Note

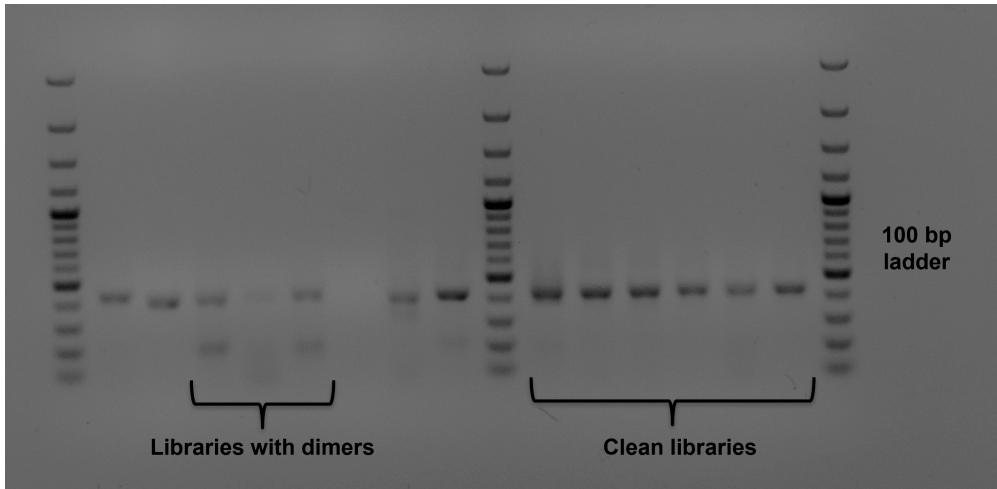

Examples of clean and primer dimer containing libraries.

Fragment size should be considered in the case of pooling to be sure about the equal sequencing depth of individual samples. Fragment size should be considered in the case of pooling to be sure about the equal sequencing depth of individual samples. Fragment size should be considered in the case of pooling to be sure about the equal sequencing depth of individual samples. Fragment size should be considered in the case of pooling to be sure about the equal sequencing depth of individual samples. Fragment size should be considered in the case of pooling to be sure about the equal sequencing depth of individual samples. Fragment size should be considered in the case of pooling to be sure about the equal sequencing depth of individual samples. Fragment size should be considered in the case of pooling to be sure about the equal sequencing depth of individual samples.

Pooling and loading final libraries

- 17 Fragment size should be considered in the case of pooling to be sure about the equal sequencing depth of individual samples.
- 17.1 Pool all samples together in a  1.5 mL Eppendorf Low Binding tube in equimolar concentration.



17.2 Dilute the pooled libraries in RSB to 100 pM final concentration. Add PhiX control.

17.3 Load  20 μ L onto an iSeq 100 2×150 bp flow cell.

17.4 Start the sequencing.



Protocol references

Amplicon based targeted sequencing:

Quick, J., Grubaugh, N. D., Pullan, S. T., Claro, I. M., Smith, A. D., Gangavarapu, K., Oliveira, G., Robles-Sikisaka, R., Rogers, T. F., Beutler, N. A., Burton, D. R., Lewis-Ximenez, L. L., de Jesus, J. G., Giovanetti, M., Hill, S. C., Black, A., Bedford, T., Carroll, M. W., Nunes, M., ... Loman, N. J. (2017). Multiplex PCR method for MinION and Illumina sequencing of Zika and other virus genomes directly from clinical samples. *Nature Protocols*, 12(6). <https://doi.org/10.1038/nprot.2017.066>

ARTIC SARS-CoV-2 sequencing protocol v4 (LSK114) V.4

DOI: [dx.doi.org/10.17504/protocols.io.bp2l6n26rgqe/v4](https://doi.org/10.17504/protocols.io.bp2l6n26rgqe/v4)

<https://www.protocols.io/view/artic-sars-cov-2-sequencing-protocol-v4-lsk114-bp2l6n26rgqe/v4>

Koskela von Sydow, A., Lindqvist, C. M., Asghar, N., Johansson, M., Sundqvist, M., Mölling, P., & Stenmark, B. (2023). Comparison of SARS-CoV-2 whole genome sequencing using tiled amplicon enrichment and bait hybridization. *Scientific Reports*, 13(1). <https://doi.org/10.1038/s41598-023-33168-1>

Vogels, C. B. F., Hill, V., Breban, M. I., Chaguza, C., Paul, L. M., Sodeinde, A., Taylor-Salmon, E., Ott, I. M., Petrone, M. E., Dijk, D., Jonges, M., Welkers, M. R. A., Locksmith, T., Dong, Y., Tarigopula, N., Tekin, O., Schmedes, S., Bunch, S., Cano, N., ... Grubaugh, N. D. (2024). DengueSeq: a pan-serotype whole genome amplicon sequencing protocol for dengue virus. *BMC Genomics*, 25(1). <https://doi.org/10.1186/s12864-024-10350-x>

AmpliSeq for Illumina SARS-CoV-2 Research Panel

<https://emea.illumina.com/products/by-brand/ampliseq/community-panels/sars-cov-2.html>

Usutu virus (USUV):

Amplicon based targeted sequencing for USUV: